

Hanford Radiological Protection Support Services Annual Report for 2000

T. P. Lynch
D. E. Bihl
M. L. Johnson

J. A. MacLellan
R. K. Piper

May 2001

Prepared for the U.S. Department of Energy
under Contract DE-AC06-76RL01830

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor Battelle Memorial Institute, nor any of their employees, makes **any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights.** Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or Battelle Memorial Institute. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

PACIFIC NORTHWEST NATIONAL LABORATORY

operated by

BATTELLE

for the

UNITED STATES DEPARTMENT OF ENERGY

under Contract DE-AC06-76RL01830

Printed in the United States of America

Available to DOE and DOE contractors from the
Office of Scientific and Technical Information,

P.O. Box 62, Oak Ridge, TN 37831-0062;

ph: (865) 576-8401

fax: (865) 576-5728

email: reports@adonis.osti.gov

Available to the public from the National Technical Information Service,
U.S. Department of Commerce, 5285 Port Royal Rd., Springfield, VA 22161

ph: (800) 553-6847

fax: (703) 605-6900

email: orders@ntis.fedworld.gov

online ordering: <http://www.ntis.gov/ordering.htm>



This document was printed on recycled paper.

**Hanford Radiological
Protection Support Services
Annual Report for 2000**

T. P. Lynch	J. A. MacLellan
D. E. Bihl	R. K. Piper
M. L. Johnson	

May 2001

Prepared for
the U.S. Department of Energy
under Contract DE-AC06-76RL01830

Pacific Northwest National Laboratory
Richland, Washington 99352

Summary

During calendar year (CY) 2000, the Pacific Northwest National Laboratory (PNNL) performed its customary radiological protection support services in support of the U.S. Department of Energy (DOE) Richland Operations Office (RL) and the Hanford contractors. These services included 1) external dosimetry, 2) internal dosimetry, 3) in vivo measurements, 4) radiological records, 5) instrument calibration and evaluation, and 6) calibration of radiation sources traceable to the National Institute of Standards and Technology (NIST). The services were provided under a number of programs as summarized here.

The Hanford External Dosimetry Program (HEDP) supports Hanford radiation protection programs by providing external radiation monitoring capabilities for all Hanford workers and visitors to help ensure their health and safety. The HEDP also provides sitewide nuclear accident and environmental dosimetry services. The 43,760 dose results reported in CY 2000 represented a 3% increase from CY 1999. The HEDP successfully passed the DOE Laboratory Accreditation Program (DOELAP) performance testing criteria for all 36 requested categories. In addition, only a single finding resulted from the National Voluntary Laboratory Accreditation Program onsite assessment this year. Several changes were implemented or initiated during the year. These included improved tracking of dosimeters in process, improved documentation of dose adjustments, evaluation of incorrect filter thickness in dosimeter holders, development of a new neutron algorithm for estimating dose from neutrons at the Plutonium Finishing Plant, and evaluation of the deep dose response of the Hanford standard dosimeter to energetic beta radiation. Technical studies were performed in the areas of code development, uncertainty analysis, dosimeter filters, dosimeter response for specific exposure geometries, and ^{32}P analyses to estimate doses from a criticality event.

The Hanford Internal Dosimetry Program (HIDP) provides for the assessment and documentation of occupational dose from intakes of radionuclides at the Hanford Site. The 5,369 excreta bioassay measurements performed in CY 2000 were slightly greater than the number performed in CY 1999. Major revisions were made to the technical basis manual that describes the bases for the internal dose calculations performed at Hanford and the new revision was issued in CY 2000. The decision level used for alpha spectrometry was revised. The bioassay analytical contract was novated to a new company. The excreta bioassay contractor experienced problems with a backlog of alpha spectrometry samples and excessive ^{243}Am false positives during the year. Dose assessments were performed for the 21 incidents that occurred with the potential for an intake. One hundred three evaluations were started because of routine bioassay results that exceeded the criteria for investigation. Six assessments of the HIDP were conducted during the year. Four technical studies were performed to 1) determine the dose from tritium absorption through the skin, 2) investigate a new internal dosimetry code, 3) review historical records in the radiological exposure (REX) system, and 4) establish a bioassay program for firefighters. A draft basic ordering agreement for a DOE-wide in vitro bioassay contract was reviewed.

The In Vivo Monitoring Program provides the in vivo counting services for radiation workers at the Hanford Site. The 6,983 in vivo measurements performed in CY 2000 represented a 14% decrease from the 8,085 measurements performed in CY 1999. The first full year of operation with the Abacos software was completed. Technical equivalence was granted by DOELAP for the new Abacos software system.

Subsequently, the DOELAP performance test criteria were met for all six categories for which reaccreditation was requested. The DOELAP onsite assessment was completed in January 2001. The performance of the standup counter was improved. The portable planar high-purity germanium counting system was calibrated for low- and high-energy applications. A spare whole body counting system was installed in the Lead Room. Digital signal processing electronics were installed in one counting room. Technical studies were conducted to 1) assess the capability to measure iodine in the thyroid, 2) study the impact of medically administered radionuclides on counting systems, 3) assess coincidence summing effects for lung counting calibrations, 4) evaluate the impact of platinum X-rays on check source quality, and 5) generate a computer model of a check source geometry.

The Hanford Radiation Records Program preserves and administers all Hanford records of personnel radiological exposure, historical radiation protection, and radiological dosimetry practices and policies. It also produces reports for DOE Headquarters, RL, the Office of River Protection, Hanford contractors, individuals, and other authorized agencies, and it provides data for epidemiology and research projects. The total number of reports issued in CY 2000 was similar to the CY 1999 total. The 50,000 documents scanned and indexed were 50% higher in number compared to the CY 1999 number. The Access Control Entry System software was upgraded in May and work started later in the year on the next revision. The REX database was redesigned, moved to a new platform, and put into production in October. The LaserCAL system operated for the full year as the document database for the Instrumentation Services and Technology Program.

The Instrumentation Services and Technology Program (IS&TP) provides complete and reliable radiation protection instrument services for site contractors to ensure personnel safety in the Hanford workplace. This includes administering the portable instrument pool for the site and supporting the Hanford Instrument Evaluation Committee. It was determined that the age of instruments in the pool does not appear to be adversely affecting performance. The 14,546 calibrations performed in CY 2000 represents a slight increase from the number of calibrations performed in CY 1999. The IS&TP assumed responsibility for managing the Maintenance and Test Equipment project in CY 2000.

The Radiation Standards and Calibration Program maintains the radiological standards necessary to support the characterization and calibration needs of instrument and external dosimetry projects. The radiological reference fields maintained include gamma, beta, and neutron isotopic sources and X-ray-generating devices. Maintaining radiological reference fields traceable to national standards is a primary goal for the program. In CY 2000, verification measurements were made of reference radiation fields' quantity and quality. The accuracy of instrument standards was also verified during the year. Exposures were made of Hanford dosimeters to support audit and quality control evaluations. The full bremsstrahlung X-ray capability was restored. Repair of the two Phillips X-ray systems was completed. Characterization of the ^{204}Tl beta source continued in CY 2000. Five audits of the program were conducted during the year.

Abbreviations and Acronyms

ACES	Access Control Entry System
ACLS	Administrative Control Limits
AIC	air-equivalent ionization chamber
AMAD	activity median aerodynamic diameter
ANSI	American National Standards Institute
BEGe	broad energy germanium
BHI	Bechtel Hanford Incorporated
BOA	basic ordering agreement
CAM	continuous air monitor
CAR	computer-assisted retrieval (system)
CC	coaxial (high-purity germanium) counter
CD	compact disc
CEDE	committed effective dose equivalent
CFR	Code of Federal Regulations
CHG	CH2M Hill Hanford Group, Inc.
CR&A	Calibration Research and Accreditation (subgroup)
CWT	chest-wall thickness
CY	calendar year
D ₂ O	deuterated water
DEC	Digital Equipment Corporation
DNFSB	Defense Nuclear Facility Safety Board
DOE	U.S. Department of Energy
DOELAP	DOE Laboratory Accreditation Program
DSP	digital signal processing
ERC	Environmental Restoration Contractor (team)
E _{res}	maximum residual energy
FA	failed analysis
FH	Fluor Hanford, Inc.
FOIA	Freedom of Information Act
FY	fiscal year
GM	Geiger-Müller
HCND	Hanford combination neutron dosimeter
HEDP	Hanford External Dosimetry Program

HEHF	Hanford Environmental Health Foundation
HIDP	Hanford Internal Dosimetry Program
HIEC	Hanford Instrument Evaluation Committee
HLAN	Hanford Local Area Network
HPDAC	Hanford Personnel Dosimetry Advisory Committee
HPGe	high-purity germanium
HPS	Health Physics Society
HQ	Headquarters
HRRP	Hanford Radiological Records Program
HSD	Hanford standard dosimeter
HVL	half-value layer
IAEA	International Atomic Energy Agency
IARC	International Agency for Research on Cancer
ICRP	International Commission on Radiological Protection
ID	identifier
IMBA	Integrated Modules for Bioassay Analysis (Code)
IODR	Investigation of Dosimetry Result
IPUL	low-level isotopic plutonium
IR	Iron Room
IS	insufficient sample volume
ISO	International Standards Organization
IS&TP	Instrumentation Services and Technology Program
IVMP	In Vivo Monitoring Program
IVRRF	In Vivo Radioassay and Research Facility
LaserCAL	CD-ROM imaging system for calibration records
LaserREX	CD-ROM imaging subsystem to REX
L _c	decision level
LC	lost container
LEPD	low-energy photon detector
LMSI	Lockhead Martin Services, Inc.
LSR	Low-Scatter Room
MCA	multichannel analyzer
MCNP	Monte Carlo N-Particle (transport code)
MDA	minimal detectable activity
MQA	measurement quality assurance
M&TE	Measuring and Test Equipment (calibration project)
NA	not applicable
NBS	National Bureau of Standards
ND	kit not delivered
NIM	nuclear instrument module

NIOSH	National Institute for Occupational Safety and Health
NIST	National Institute of Standards and Technology
NRPB	National Radiation Protection Board (United Kingdom)
NS	no sample received
NVLAP	National Voluntary Laboratory Accreditation Program
ORP	Office of River Protection
PAAA	Price Anderson Act Amendment
PC	personal computer
PFP	Plutonium Finishing Plant
PMT	photomultiplier tube
PNNL	Pacific Northwest National Laboratory
PTB	Physikalisch-Technische Bundesanstalt
PTW	Physikalisch-Technische Werkstätten
QA	quality assurance
QC	quality control
REX	Radiological Exposure (system)
R&HT	Radiation and Health Technology
RL	U.S. Department of Energy Richland Field Office
RPG	Radiochemistry Process Group
RS&CP	(Hanford) Radiation Standards and Calibrations Program
RWP	Radiation Work Permit
SAIC	Science Applications International Corporation
SOW	Statement of Work
SS	Stainless Steel Room
STL	Severn Trent Laboratories
SU	standup counter
TIBM	thoron in-breath monitor
TL	thermoluminescent (dosimetry)
TLD	thermoluminescent dosimeter
TPU	total propagated uncertainty
TRIP	Thyroid Radioiodine Intercomparison Program
TRU	transuranium radionuclide(s)
URL	uniform resource locator
USE	U.S. Ecology
WB	whole body
WBC	whole body count

Y2K

Year 2000

Contents

Summary	iii
Abbreviations and Acronyms	v
1.0 Introduction	1.1
2.0 Hanford External Dosimetry Program.....	2.1
2.1 Routine Operations.....	2.2
2.2 Program Changes and Improvements.....	2.4
2.2.1 Tracking Status of Dosimeters in Process	2.4
2.2.2 Improvement in Documentation of Dose Adjustments	2.4
2.2.3 Incorrect Tin Filter Thickness in HSD Holders	2.4
2.2.4 New 8816 Algorithm for Plutonium Finishing Plant Neutrons Proposed.....	2.5
2.2.5 Deep Dose in HSDs From Beta-Radiation-Only Fields.....	2.5
2.2.6 Effects of the Millennium Transition	2.5
2.3 Program Assessments and Quality Assurance	2.6
2.3.1 Blind Audit Personnel Dosimeters	2.6
2.3.2 Blind Audit Environmental Dosimeters	2.6
2.3.3 Department of Energy Laboratory Accreditation Program	2.6
2.3.4 National Voluntary Laboratory Accreditation Program.....	2.11
2.3.5 Energy Northwest Assessment.....	2.12
2.3.6 Self-Assessments.....	2.12
2.3.7 Environmental Dosimeter Intercomparison	2.12

2.4	Supporting Technical Studies.....	2.12
2.4.1	New External Dosimetry Code.....	2.13
2.4.2	Evaluation of Lead Impurity in Tin Filters in the 8825 Holders.....	2.13
2.4.3	Uncertainty Analyses	2.13
2.4.4	Effect of Lead Aprons on Response of 8825 and 8816 Dosimeters.....	2.13
2.4.5	Analysis of Phosphorus-32 in Sulfur Pellets and Hair	2.14
2.4.6	Shallow Dose Rate from T-Handle Waste Sample Carriers.....	2.14
2.5	Skin Contaminations	2.15
2.6	Program-Related Professional Activities	2.15
2.6.1	Activities	2.15
2.6.2	Presentations.....	2.16
2.6.3	Publications	2.16
2.6.4	Professional Memberships	2.16
3.0	Hanford Internal Dosimetry Program.....	3.1
3.1	Routine Operations.....	3.1
3.1.1	Bioassay Capabilities	3.2
3.1.2	Excreta Bioassay Contract Activities	3.3
3.1.3	Excreta Bioassay Monitoring Activities.....	3.4
3.1.4	Potential Intake Evaluations.....	3.9
3.2	Program Changes and Improvements.....	3.12
3.2.1	Methods and Models Manual Issued.....	3.12
3.2.2	Changes to the Hanford Internal Dosimetry Program Manual.....	3.12

3.2.3	Update on New Decision Level for Alpha Spectrometry.....	3.12
3.3	Program Assessments.....	3.13
3.3.1	Excreta Quality Control Oversight Program.....	3.13
3.3.2	Onsite Inspection of the Excreta Contract Laboratory	3.14
3.3.3	Testing of Backup Lab for Rapid Plutonium and Strontium Analyses	3.14
3.3.4	Hanford Contractors' 10 CFR 835 Assessment	3.14
3.3.5	Program Self-Assessments.....	3.15
3.3.6	Quality Problem Reports.....	3.15
3.4	Supporting Technical Studies.....	3.16
3.4.1	Tritium Absorption Through Skin.....	3.16
3.4.2	Investigation of a New Internal Dosimetry Code.....	3.16
3.4.3	Review of Historical Records on REX.....	3.17
3.4.4	Bioassay for Hanford Firefighters.....	3.17
3.4.5	Review of Draft Basic Ordering Agreement.....	3.17
3.5	Project-Related Professional Activities.....	3.17
3.5.1	Activities	3.18
3.5.2	Presentations.....	3.18
3.5.3	Publications	3.18
3.5.4	Professional Memberships and Other Activities	3.18
4.0	In Vivo Monitoring Program for Hanford.....	4.1
4.1	Routine Operations.....	4.1
4.1.1	Program Documentation	4.3

4.1.2	Department of Energy Laboratory Accreditation Program	4.4
4.1.3	Equipment Maintenance and Repair	4.5
4.1.4	Facility-Related Activities.....	4.6
4.1.5	Historical In Vivo Measurement Records	4.6
4.2	Program Changes and Improvements.....	4.6
4.3	Program Assessments.....	4.7
4.4	Supporting Technical Studies.....	4.7
4.4.1	Thyroid Radioiodine Intercomparison Program.....	4.8
4.4.2	Thoron In-Breath Monitor Study	4.8
4.4.3	Measurement Quality Control	4.8
4.4.4	Measurements of Thallium Following Medical Administration	4.9
4.4.5	$^{241}\text{Am}/^{152}\text{Eu}$ Lung Phantom and Coincidence Summing	4.10
4.4.6	Check Source Anomaly.....	4.11
4.5	Program-Related Professional Activities	4.11
4.5.1	Activities	4.12
4.5.2	Presentations.....	4.12
4.5.3	Publications	4.12
5.0	Hanford Radiation Records Program.....	5.1
5.1	Overview	5.1
5.1.1	Database Administration	5.1
5.1.2	Data Processing	5.2
5.1.3	Report Issuance	5.2

5.1.4	Records Library.....	5.2
5.2	Routine Operations.....	5.3
5.2.1	Data Administration.....	5.3
5.2.2	Data Processing.....	5.3
5.2.3	Report Issuance.....	5.4
5.2.4	Records Library.....	5.7
5.3	Program Changes and Improvements.....	5.7
5.3.1	ACES Database.....	5.7
5.3.2	REX Database.....	5.7
5.3.3	Document Scanning.....	5.8
5.4	Program Assessment.....	5.8
5.5	Supporting Projects.....	5.8
5.6	Program-Related Professional Activities.....	5.9
6.0	Instrumentation Services and Technology Program.....	6.1
6.1	Routine Operations.....	6.1
6.1.1	Administration of the Portable Instrument Pool.....	6.1
6.1.2	Calibration and Maintenance Service.....	6.2
6.1.3	Calibration As-Founds Out-of-Tolerance.....	6.8
6.1.4	Maintenance of the Calibration Records.....	6.9
6.2	Program Improvements in Calibration and Maintenance Operations.....	6.9
6.3	Hanford Instrument Evaluation Committee.....	6.9
6.4	Supporting Technical Studies.....	6.10

6.5	Program-Related Professional Activities	6.10
6.5.1	Presentations.....	6.10
6.5.2	External Professional Activities	6.10
7.0	Radiation Standards and Calibrations Program.....	7.1
7.1	Routine Operations.....	7.1
7.1.1	Standards and Capabilities	7.1
7.1.2	Traceability to National Standards	7.8
7.1.3	Quantitative and Qualitative Confirmation of Standards	7.13
7.1.4	Applications	7.16
7.2	Operational Improvements.....	7.17
7.2.1	Repair/Replacement of X-Ray Systems	7.17
7.3	Program Assessments.....	7.21
7.4	Project-Related Professional Activities.....	7.22
7.4.1	Presentations.....	7.22
7.4.2	Publications	7.23
7.4.3	External Professional Activities	7.23
8.0	References	8.1

Figures

1.1	Management Structure and Major Communication Interfaces for Hanford Radiation Protection Services since October 2000	1.2
2.1	Trend in Reported Hanford Personnel Dosimeter Results.....	2.2
2.2	DOELAP Performance Test Results for the HSD Whole Body Dosimeter, Deep Dose.....	2.8
2.3	DOELAP Performance Test Results for the HSD Whole Body Dosimeter, Shallow Dose.....	2.9
2.4	DOELAP Performance Test Results for the HCND Whole Body Dosimeter, Deep Dose	2.9
2.5	DOELAP Performance Test Results for the HCND Whole Body Dosimeter, Shallow Dose...	2.10
2.6	DOELAP Performance Test Results for the Hanford Ring Dosimeter, Shallow Dose	2.10
2.7	DOELAP Performance Test Results for the HSD Wrist Dosimeter, Shallow Dose	2.11
3.1	Standard and Nonstandard Excreta Requests by Month for 2000	3.6
3.2	Routine Urine Measurements Made from 1994 Through 2000.....	3.6
3.3	Excreta Samples Not Obtained in the Grace Period	3.8
3.4	Termination Excreta Samples Not Obtained	3.8
3.5	Number of Open Evaluations by Month.....	3.11
4.1	Summary of the Number and Types of In Vivo Measurements Performed from 1991 Through 2000.....	4.3
4.2	Lung Phantom Quality Control Results.....	4.9
4.3	²⁰¹ Ti Net Peak Count Rate at 167 keV.....	4.9
4.4	²⁰² Ti Count Rate Versus Time After Injection.....	4.10
4.5	Efficiency Calibration Comparison	4.11
5.1	Number of Requests for Previous Exposure.....	5.5
5.2	Number of Responses to Requests for Previous Exposure.....	5.5
5.3	Number of Visitor Exposure Letters.....	5.6
5.4	Number of Termination Letters	5.6
5.5	Number of Documents Scanned/Indexed	5.6
6.1	Total Number of Calibrations for Hanford Clients During CY 2000.....	6.8
7.1	GB650 ⁶⁰ Co Irradiator	7.4
7.2	Example Spectrum of X-Ray Configurations.....	7.5
7.3	Typical Traceability Pathway for PNNL Photon Reference Fields.....	7.10
7.4	Typical Traceability Pathway for PNNL Neutron Reference Fields.....	7.11
7.5	Typical Traceability Pathway for PNNL Beta Reference Fields.....	7.13
7.6	Reduction in K-Fluorescence Exposure Rates Due to Addition of Primary Filter.....	7.18
7.7a	Effect of Primary Filter on 17.5-keV K-Fluorescence Spectra	7.19
7.7b	Effect of Primary Filter on 59.3-keV K-Fluorescence Spectra	7.19
7.8	Comparison of New and Old ²⁰⁴ Ti Source Transmission	7.20

Tables

2.1	External Whole Body Doses Received by Hanford Workers in 2000.....	2.3
2.2	Audit Dosimeters Processed During 2000.....	2.6
2.3	DOELAP Whole Body Performance Test Data	2.7
2.4	DOELAP Extremity Dosimeters Shallow-Dose Performance Test Data.....	2.8
2.5	Number of Skin Contaminations	2.15
3.1	Specified Minimum Detectable Activities and Screening Levels for Routine Excreta Analyses During CY 2000.....	3.3
3.2	Minimum Detectable Activities and Screening Levels for Routine In Vivo Measurements During CY 2000	3.4
3.3	Specified Minimum Detectable Activities for Emergency and Expedited Excreta Bioassay During CY 2000	3.5
3.4	Worker Excreta Measurements Reported in 2000.....	3.7
3.5	Summary of Potential Intake Incidents During 2000	3.9
3.6	Summary of Intake Cases Identified Through the Routine Bioassay Program During 2000....	3.10
3.7	Comparison of Potential Intakes by Reason Code, 1994 to 2000	3.10
3.8	Range of New Internal Doses Assigned to the Hanford Work Force in 2000.....	3.11
3.9	Changes to the <i>Hanford Internal Dosimetry Program Manual</i>	3.13
4.1	In Vivo Measurements Performed During 2000 and Entered in the REX Database.....	4.2
4.2	In Vivo Count Summary from 1991 Through 2000	4.2
4.3	Results from CY 2000 DOELAP Performance Testing	4.4
4.4	Results from the Thyroid Radioiodine Intercomparison Program.....	4.8
5.1	Data Processing Center Activity for Calendar Year 2000.....	5.4
5.2	Number of Responses to Requests for Previous Exposure.....	5.4
5.3	Number of Visitor Exposure Letters.....	5.5
6.1	Instrument Calibrations by Unit-Price Category and by Calendar Year	6.2
6.2	CY 2000 Calibration Volume for All Hanford Contractors	6.3
6.3	CY 2000 Calibration Volume for Fluor Hanford, Inc.	6.4
6.4	CY 2000 Calibration Volume for CH2M Hill Hanford Group	6.5
6.5	CY 2000 Calibration Volume for Bechtel Hanford, Inc.....	6.6
6.6	CY 2000 Calibration Volume for PNNL.....	6.7
7.1	Available Gamma-Ray Sources (1999).....	7.2
7.2a.	Available NIST-Specified Bremsstrahlung X-Ray Reference Fields (2000).....	7.6
7.2b	Available ISO-Specified Bremsstrahlung X-Ray Reference Fields (2000)	7.7
7.2c	Available K-Fluorescence Reference X-Ray Fields (2000)	7.7
7.3	Available Beta Reference Fields (2000).....	7.8
7.4	Summary of 2000 Audit Items	7.22

1.0 Introduction

Specific radiation protection services are performed routinely by the Pacific Northwest National Laboratory (PNNL)^(a) for the U.S. Department of Energy (DOE) Richland Operations Office (RL) and the Hanford Site contractors. These sitewide services are provided by programs in 1) external dosimetry, 2) internal dosimetry, 3) in vivo monitoring, 4) radiation records, 5) instrument calibration and evaluation, and 6) calibration of radiation sources traceable to the National Institute of Science and Technology (NIST). The program work is performed by staff in the Radiation and Health Technology (R&HT) technical group, which falls under the purview of the Environmental Technology Division. The R&HT group was transferred from the Process Technology organization to Systems and Risk Analysis organization on October 1, 2000.

R&HT is organized into five functional groups: 1) Dosimetry Services, 2) Instrumentation Services and Technology, 3) Radiation Records, 4) Administration, and 5) Dosimetry Research and Technology. The Dosimetry Services group includes the Hanford External Dosimetry Program, the Hanford Internal Dosimetry Program, and the In Vivo Monitoring Program, which includes the operational and technical staff at the In Vivo Radioassay and Research Facility; and the Dosimetry Operations Program, which includes all of the Dosimetry Services technician staff that perform the processing of dosimeters, handling of dosimeters, and bioassay scheduling for Fluor Hanford, Inc. (FH) and RL, and Radiological Exposure (REX) data processing (which was transferred from the Hanford Radiological Records Program). The Instrumentation Services and Technology group includes four programs: Radiological Calibration Services, Non-Radiological Calibration Services, Instrument Repair, and Instrument Testing and Qualification. The Hanford Radiation Records Program includes the Records Library, Exposure Reporting, and Data Administration tasks. Information Services policy and planning for R&HT are assigned to a staff position reporting directly to the R&HT manager. The Administration group is responsible for financial planning and secretarial support.

Although some of the programs described in this report are involved in activities funded by other sources, only those activities funded by RL, DOE-Headquarters (HQ), or the Hanford contractors are addressed here. Services provided for non-RL activities are performed only to the extent that they do not adversely affect services to DOE and its contractors. These non-RL services provide funds that support the overall program and reduce costs to RL and to the Hanford contractors.

Each of the six primary programs of R&HT is described in a separate chapter of this report: 1) the Hanford External Dosimetry Program, 2) the Hanford Internal Dosimetry Program, 3) the In Vivo Monitoring Program, 4) the Hanford Radiation Records Program, 5) the Hanford Instrumentation Services and Technology Program, and 6) the Hanford Radiation Standards and Calibrations Program. Program descriptions include:

- the routine operations

(a) Pacific Northwest National Laboratory is operated by Battelle Memorial Institute for the U.S. Department of Energy under Contract DE-AC06-76RL01830.

- program changes and improvements
- program assessments
- other program-related activities, such as publications, presentations, and professional memberships.

During calendar year (CY) 2000, the Hanford contractors consisted of PNNL, Bechtel Hanford, Inc. (BHI, also referred to as the Environmental Restoration Contract [ERC] team), the Hanford Environmental Health Foundation (HEHF), FH, and CH2M-Hill Hanford Group (CHG). FH consists of these five primary projects: Spent Nuclear Fuel, Waste Management, Nuclear Material Stabilization, River Corridor, and the Fast Flux Test Facility.

The PNNL and RL management structure and communication interfaces for each PNNL-operated program are shown in the organizational chart in Figure 1.1. The RL Office of Site Services is now responsible for PNNL services in this area.

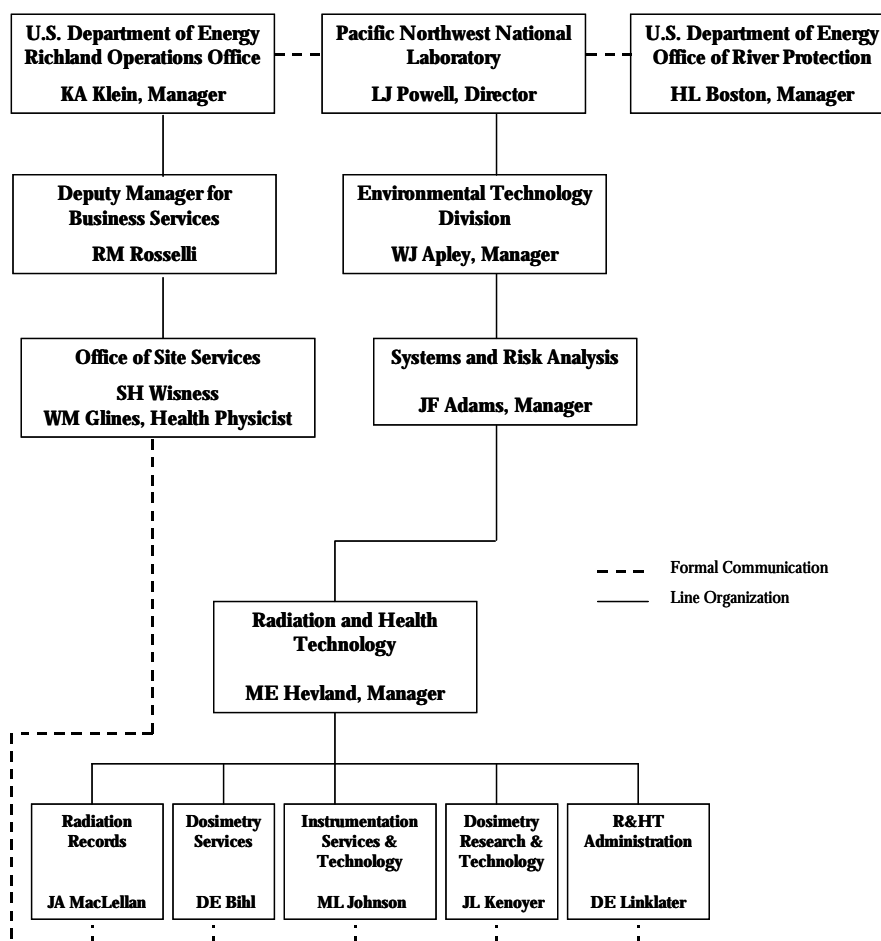


Figure 1.1. Management Structure and Major Communication Interfaces for Hanford Radiation Protection Services since October 2000

2.0 Hanford External Dosimetry Program

The Hanford External Dosimetry Program (HEDP) provides the official dose from external radiation for all Hanford personnel in support of Hanford radiation protection programs. (The program is available for use by other DOE sites or non-DOE customers as well.) HEDP dosimeter results provide the means used by contractor personnel to project, control, and measure radiation doses received by personnel. The program also provides sitewide nuclear accident, environmental, and building area dosimetry. The program operates in compliance with DOE requirements as set forth in 10 CFR 835, *Occupational Radiation Protection*, and it is accredited by both the DOE Laboratory Accreditation Program (DOELAP) and the Department of Commerce National Voluntary Laboratory Accreditation Program (NVLAP).

The Hanford whole body personnel dosimetry system consists of a commercially procured thermoluminescent (TL) dosimetry system (manufactured by Bicorn/Harshaw).^(a) Dosimeters include the Hanford standard dosimeter (HSD), the Hanford combination neutron dosimeter (HCND), an extremity dosimeter, and the Hanford environmental dosimeter. The HCND also has the provision for a CR39 track-etch dosimeter, although the track-etch dosimeter was not used for personnel in 2000. The HSD also has a neutron response capability that will detect exposure to neutron radiation. Beginning in 1999, after receiving accreditation in 1998, the HSD was considered acceptable for monitoring neutron exposures, nominally below 100 mrem, with the understanding that the HSD will over-respond to low-energy neutrons. The Hanford extremity personnel dosimetry system consists of a commercially procured Bicorn/Harshaw “chipstrate” extremity dosimeter insert enclosed in an ICN/MeasuRing^(b) ring casing (DOE contractors only). The HSD is also used as an extremity (wrist or ankle) dosimeter. Both the HSD and the HCND are used for monitoring areas, the HCND being mounted on 19-L (5-gal) water-filled carboys.

Physical and functional details about the HSD, HCND, finger ring, and the environmental dosimeter are provided in the *Hanford External Dosimetry Technical Basis Manual*.^(c) Additional details about program operation are documented in the *Hanford External Dosimetry Quality Manual*,^(d) the *Hanford*

(a) Bicorn/Harshaw, Saint-Gobain/Crystals and Detectors, Solon, Ohio.

(b) ICN Biomedicals, Inc., Costa Mesa, California.

(c) Pacific Northwest National Laboratory. 2000. *Hanford External Dosimetry Technical Basis Manual*. PNL-MA-842, Richland, Washington. (Internal manual.) Available URL: <http://www.pnl.gov/eshs/pub/pnl842.html>

(d) Pacific Northwest National Laboratory. 1998. *Hanford External Dosimetry Quality Manual*. PNL-MA-859, Richland, Washington. (Internal manual.)

External Dosimetry Project Procedures Manual,^(a) the *Quality Assurance Plan for Hanford External Dosimetry*,^(b) and the *Hanford External Dosimetry Program Data Management Manual*.^(c)

2.1 Routine Operations

During 2000, 43,760 official personnel dose results were reported for Hanford customers. This processing volume represented a 3% increase from the total of 42,622 during 1999, essentially a leveling-off after several years of decreases. The annual number of dose results is illustrated in Figure 2.1 for 1996 through 2000 for each type of dosimeter. The use of HSDs continued to decline in 2000, decreasing 6% from 1999, but the use of HCNDs and finger rings increased (11% and 14%, respectively). The reduction in HSDs continues a trend from 1996 resulting primarily from reducing the dosimeter exchange frequency for many workers (e.g., from monthly to quarterly and quarterly to annual). The numbers in Figure 2.1 do not include internal quality control (QC) dosimeter cards or cards processed in support of DOELAP testing, and each HCND counts as one even though there really are two dosimeters in the packet.

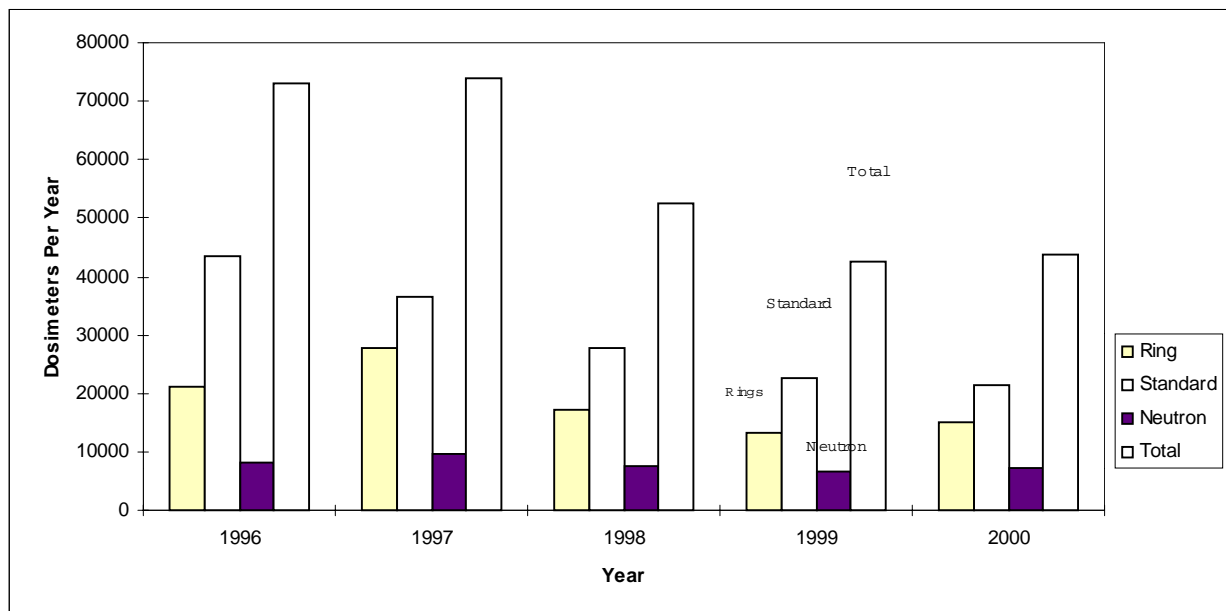


Figure 2.1. Trend in Reported Hanford Personnel Dosimeter Results

-
- (a) Pacific Northwest National Laboratory. Current version. *Hanford External Dosimetry Project Procedures Manual*. PNNL-MA-841, Richland, Washington. (Internal manual.)
- (b) Pacific Northwest National Laboratory. Current version. *Quality Assurance (QA) Plan*. No. LSC-022, Richland, Washington. (Internal document.)
- (c) Pacific Northwest National Laboratory. Current version. *Hanford External Dosimetry Program Data Management Manual*. PNL-MA-844, Pacific Northwest National Laboratory, Richland, Washington. (Internal manual.)

As in previous years, the CR39 track-etch capability of the HCND was not used. This action was recommended by the Hanford Personnel Dosimetry Advisory Committee (HPDAC) and was based on the relatively low-energy neutron spectra at the Plutonium Finishing Plant (PFP). Plutonium at PFP is primarily being stored awaiting DOE decisions about its eventual disposition. As such, the neutron energy spectra are greatly moderated because of the extensive shielding, and the neutrons are primarily less energetic than the approximate 100-keV energy threshold of the track-etch foil. This assumption was verified by a study performed in 1999 (Scherpelz, Fix, and Rathbone 2000).

Statistical tracking of dosimeters that were issued then subsequently lost or not returned for whatever reason was renewed in 1998 after being suspended for a couple of years. Because there are lag periods before unreturned dosimeters are declared lost, not all potentially lost dosimeters are included in these statistics. The lag periods are 60 days for monthly exchanged dosimeters, 180 days for quarterly exchanged dosimeters, and 465 days for annually exchanged dosimeters. The numbers of dosimeters declared lost in 2000 were as follows: 70 HSDs, 18 HCNDs, 134 finger rings, and 16 area dosimeters.

Statistics on external whole body doses received by the Hanford workforce are provided in Table 2.1. The total number of monitored workers was 9,689 in 2000, a 3% decrease from 1999. The highest external dose for an individual worker was 1,407 mrem in 2000, which was comparable to the highest dose of 1,499 mrem in 1999. The number of workers in the 1,000- to 1,999-mrem range has increased each year from 3 in 1998 to 32 in 2000.

Table 2.1. External Whole Body Doses Received by Hanford Workers in 2000^(a)

Dose Range (mrem)	Number of Workers in Dose Range							
	BHI	FH	CHG	PNNL	DOE^(b)	HEHF^(c)	Other	Total
Zero	887	3,274	832	1,194	852	28	711	7,778
1-99	85	782	214	131	15	0	154	1,381
100-249	18	159	66	20	1	0	28	292
250-499	2	95	25	18	0	0	10	150
500-749	1	32	1	3	0	0	0	37
750-999	0	19	0	0	0	0	0	19
1000-1999	0	32	0	0	0	0	0	32
>2000	0		0	0	0	0	0	0
(a) For monitored workers.								
(b) Includes Office of River Protection.								
(c) HEHF = Hanford Environmental Health Foundation.								

There were 606 Investigation of Dosimeter Results (IODRs) processed related to doses incurred in 2000 (DOE—22, FH—414, CHG—79, BHI—69, and PNNL—22).

In addition to personnel dosimeters, the HEDP also processed 1,629 area dosimeters, 880 environmental dosimeters, and 86 fixed nuclear accident dosimeters. The number of environmental dosimeters increased slightly compared with 1999, but the numbers of area and fixed nuclear accident dosimeters decreased slightly from 1999 and were comparable to the numbers in 1998.

2.2 Program Changes and Improvements

Major modifications to HEDP practices are discussed during HPDAC meetings. Six changes in program practices were made during 2000, as described in the following sections.

2.2.1 Tracking Status of Dosimeters in Process

Three codes were written to assess the status of dosimeters in process. `Returned_Not_Scanned_In` identifies dosimeters that have been returned in REX but have no record in our internal tracking file (with a grace period of 5 days). `Scanned_In_Not_Processed` identifies dosimeters scanned into our lab for which reader data have not been processed through completion of dose results on the VAX (with a grace period of 10 days from scan-in date). `Processed_Not_Reported` finds records in the dose file that have not been transferred to REX (with a grace period of 15 days from scan-in date). These codes are run and the output reports are reviewed weekly.

2.2.2 Improvement in Documentation of Dose Adjustments

When the thermoluminescent dosimeter (TLD) reader detects something anomalous with a glow curve (e.g., shifted, poorly shaped), the glow curve is flagged and requires review by a dosimetrist. To mark hard copies of flagged glow curves, a series of standardized notations was developed to indicate what the problem was and what method the dosimetrist used to adjust the dose from the reader-calculated value. The notations provide a consistent methodology for adjusting doses and for ease of recognition as to what method was used for each adjustment. The methodology and notations were documented in a letter to file^(a) and dosimetrists were trained on their use.

2.2.3 Incorrect Tin Filter Thickness in HSD Holders

In 1999, the manufacturer of the HSD holder notified HEDP that most holders sold since 1996 probably have tin filters that are 19-mil (0.48-mm) thick instead of being 25-mil (0.635-mm) thick, as specified. As reported in last year's report (Lynch et al. 2000, Section 2.2.5), X-ray and beta + X-ray irradiation tests were conducted on dosimeter holders that contained the thinner tin. The X-ray tests were evaluated in 1999, and the bias in dose results from the X-rays caused by the thin filters was shown to be

(a) Internal letter to file, Scott E. Huneycutt, January 31, 2000, "Glow Curve Adjustment Methodology."

inconsequential. The results of the beta + X-ray irradiation study were evaluated in 2000,^(a) and, as expected, the bias increased for the 19-mil tin relative to the 25-mil tin; however, the dosimeters met the DOELAP criteria, and the change in bias was not considered significant.

Nevertheless, a plan was implemented to remove from service over time all the holders with the 19-mil tin filters. The goal was to have no thin-tin filters in use in 2001, i.e., all dosimeter holders to be issued for use in 2001 had to be tested and the thin-tin filters removed. Complications in carrying out the plan arose when lead contamination was discovered in the tin filters, which interfered with the eddy current testing of the tin (see Section 2.4.2). However, this was overcome late in the year and the goal was met. Tested and accepted holders are now permanently marked and are also tracked in the external dosimetry database.

2.2.4 New 8816 Algorithm for Plutonium Finishing Plant Neutrons Proposed

A proposal to upgrade the algorithm applied to HCNDs used at the PFP was presented to the HPDAC in December. The proposed algorithm was developed from the neutron measurements taken at the plant in 1999 where side-by-side neutron dose measurements were obtained with HCNDs and tissue-equivalent proportional counters (Scherlpelz, Fix, and Rathbone 2000). In developing the algorithm, it was determined that there was a trade-off between obtaining an accurate response for a variety of exposure conditions that workers might encounter at the plant and reducing the variability of response between dosimeters used in similar exposure conditions. The proposed algorithm will reduce the variability in the dosimeter readings to a composite of likely exposure conditions. The proposal was under consideration by the HPDAC at year-end.

2.2.5 Deep Dose in HSDs From Beta-Radiation-Only Fields

To confirm initial indications from workplace surveys, a study was conducted to show that the HSD algorithm calculates a deep dose at about 1 to 1.5% of the shallow dose when subjected to pure beta radiation from ⁹⁰Y, whereas the true deep dose for practical purposes is zero. The study concluded that the over-response of the HSD is due to the curvature of the plastic bubble over the deep dose chip. The curvature effectively reduces the density thickness of the material overlying the chip. Algorithm changes to correct for the over-response were being drafted at year-end.

2.2.6 Effects of the Millennium Transition

Preparations conducted in the years prior to January 1, 2000, were sufficient in that there were only minor effects from the date change. The VAX cluster did have trouble restarting because of a dead battery on the disk array and two other small pieces of hardware failed to restart. These effects may have resulted more from shutting down the system for several days than from the date change. By DOE directive, constraints in place for making software changes continued until early March because of the unusual leap year.

(a) Internal letter to file, Scott E. Huneycutt, September 7, 2000, "Impact of 19-mil Tin Filter on HSD Beta Response."

2.3 Program Assessments and Quality Assurance

Each year internal audit dosimeters are processed to ensure the integrity of dosimeter processing. During 2000, 1,569 internal audit dosimeters were processed. A breakdown of the internal audit dosimeters is shown in Table 2.2.

Table 2.2. Audit Dosimeters Processed During 2000

Dosimeter Type	No. of Dosimeters
HSD	556
HCND	265
Rings	483
CR39 Track-Etch	265

Data analysis programs are used to statistically evaluate the performance for each of the audit dosimeter categories against DOELAP criteria.^(a) A QC checklist is prepared for each processing. Copies of the checklists and audit dosimeter performance reports are provided to the Hanford Radiation Protection Historical Files.

2.3.1 Blind Audit Personnel Dosimeters

FH routinely submits audit dosimeters to be processed along with the personnel dosimeters. Audit dosimeters are submitted each month of the year, and performance is analyzed each quarter for shallow, deep, and neutron dose, and dose to the finger ring dosimeters. HEDP successfully passed each of the quarterly evaluations in 2000 using DOELAP performance criteria. Documentation of HEDP results of these audits is included in the Hanford Radiation Protection Historical Files.

2.3.2 Blind Audit Environmental Dosimeters

Staff from PNNL's Surface Environmental Surveillance Program routinely submit audit dosimeters to be processed along with their quarterly exchanged environmental dosimeters. The given exposures typically range between 15 and 30 mrem of ^{137}Cs gamma radiation. For the 12 audit dosimeters submitted during 2000, the overall bias in the reported dose compared with the delivered dose was less than 0.1%, with a range in the bias of individual dosimeters from -5.5% to 10.3%. The bias plus precision statistic was 0.050. These are all excellent results. The draft environmental performance standard sets the limit for bias plus precision at 0.5.

2.3.3 Department of Energy Laboratory Accreditation Program

Performance testing of personnel dosimeters and an onsite inspection occur every 2 years for DOELAP, including 2000. Performance testing occurred from February through May. The HEDP was

(a) Audit dosimeters are processed monthly and performance reports are prepared quarterly.

tested in 36 categories, including for the HSD as an extremity dosimeter and for both the HSD and the HCND whole body dosimeters for moderated and unmoderated neutrons, with and without photons. Exposures included normal personnel and accident-level doses (as high as 500 rem) for both whole body and extremity dosimeters. In total, approximately 1000 results were submitted to the Performance Evaluation Program Administrator as part of the testing process. Whole body dosimeter performance testing followed recommendations in American National Standards Institute/Health Physics Society standard ANSI/HPS N13.11-1993, *An American National Standard, Personnel Dosimetry Performance—Criteria for Testing* (ANSI/HPS 1993), and testing of extremity dosimeters followed recommendations in HPS N13.32, *An American National Standard, Performance Testing of Extremity Dosimeters* (HPS 1995).

HEDP successfully passed all requested categories. Testing results for Hanford whole body and extremity dosimeters are summarized in Tables 2.3 and 2.4. As shown in these tables, excellent performance was obtained by the Hanford dosimeters when compared to the 0.3 or 0.4 criterion. Figures 2.2 through 2.7 illustrate the DOELAP performance for the HSD whole body dosimeter, the HCND whole body dosimeter, the Hanford ring dosimeter, and the HSD as an extremity dosimeter in the respective DOELAP categories using Horlick diagrams.

Table 2.3. DOELAP Whole Body Performance Test Data

DOELAP Category Description	DOELAP Criterion	Performance ^(a)				
		HSD		HCND		HCND with CR39
		Shallow	Deep	Shallow	Deep	Deep
High Dose, Low-Energy Photons	0.3	NA ^(b)	0.022	NA	0.052	NA
High Dose, High-Energy Photons	0.3	NA	0.026	NA	0.066	NA
Low-Energy Photons, General	0.3	0.087	0.183	0.048	0.190	NA
Low-Energy Photons, Plutonium Environments	0.3	0.188	0.184	0.128	0.166	NA
High-Energy Photons, ¹³⁷ Cs	0.3	0.047	0.004	0.057	0.026	NA
Beta Particles: General	0.3	0.021 ^(c)	NA	0.000	NA	NA
Neutron, Moderated ²⁵² Cf	0.3	NA	0.080	NA	0.015	0.069
Neutron, Unmoderated ²⁵² Cf	0.3	NA	0.039	NA	0.046	0.052
Mixtures						
Low-Energy Photons + High-Energy Photons	0.4	0.128	0.122	0.077	0.100	NA
Low-Energy Photons + Beta Particles	0.4	0.183	0.187	0.113	0.150	NA
High Energy Photons + Beta Particles	0.4	0.241	0.011	0.179	0.012	NA
Low-Energy Photons + Moderated Neutrons	0.4	NA	0.104	NA	NA	NA
High-Energy Photons + Mod. Neutrons	0.4	NA	NA	NA	0.025	NA
Low-Energy Photons + Unmod. Neutrons	0.4	NA	NA	NA	0.085	NA
High-Energy Photons + Unmod. Neutrons	0.4	NA	0.030	NA	NA	NA
(a) Performance quotients (P) for the HSD and HCND are calculated as $P = B + S - E$ where B is the bias from the known (delivered) dose, S is the standard deviation of the reported results, and E is the uncertainty in the delivered dose. Dosimeter performance quotients must be less than the DOELAP criterion in each category for satisfactory performance. (b) NA = not applicable. (c) For this category only, with ²⁰⁴ Tl beta radiation, the performance quotient is calculated as $P = B - E$.						

Table 2.4. DOELAP Extremity Dosimeters Shallow-Dose Performance Test Data

DOELAP Category Description	DOELAP Criterion	Performance ^(a)	
		Shallow	
		HSD	Ring
High Dose General Photons	0.3	0.020	0.134
Low Energy Photons	0.5	0.137	0.139
High-Energy Photons	0.5	0.031	0.076
Beta Particles, ²⁰⁴ Tl	0.5	0.082	0.204

(a) Performance quotients (P) for Hanford extremity dosimeters are calculated as $P = |B| + S$ where B is bias from the known (delivered) dose and S is the standard deviation of the reported results. Dosimeter performance quotients must be less than the DOELAP criterion in each category for satisfactory performance.

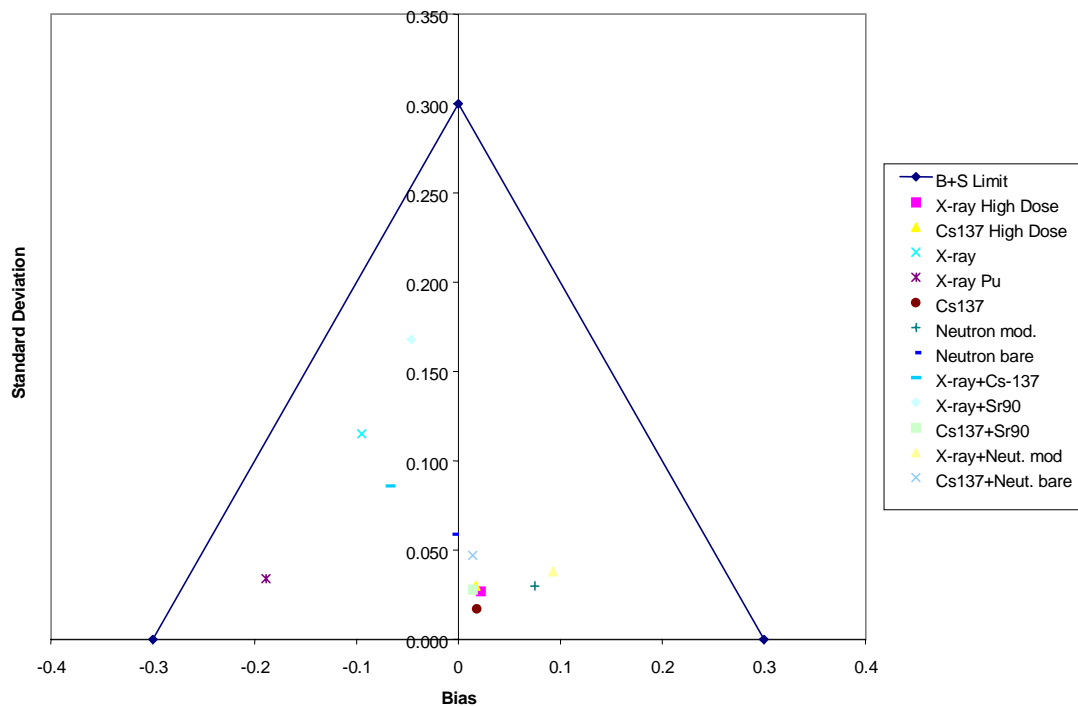


Figure 2.2. DOELAP Performance Test Results for the HSD Whole Body Dosimeter, Deep Dose

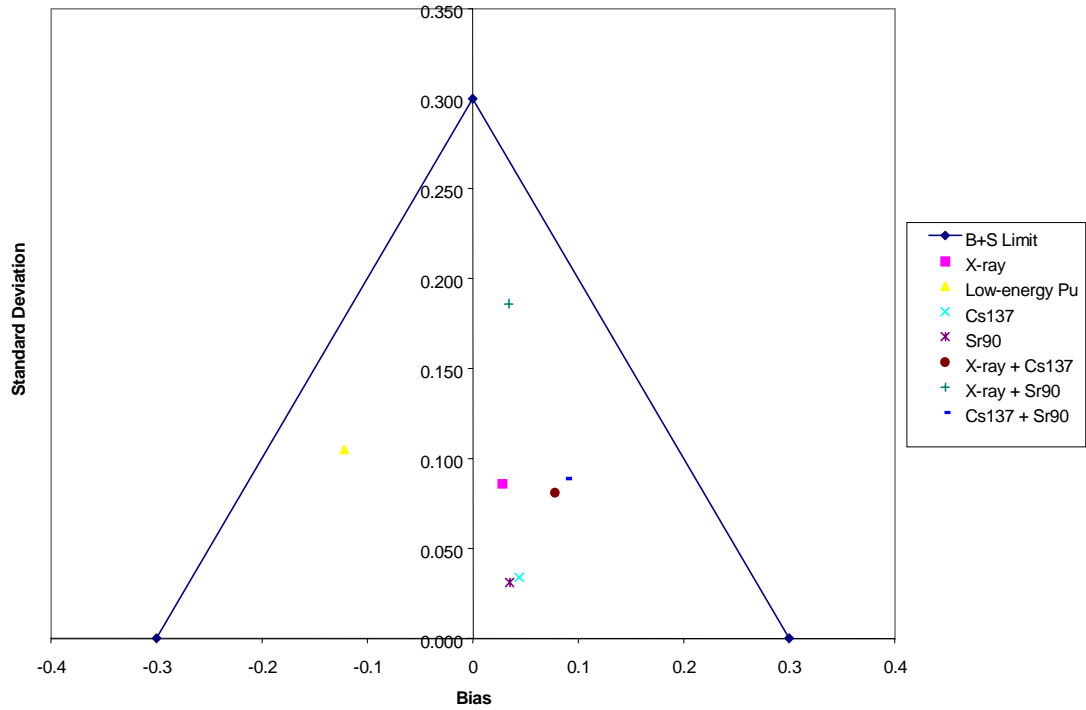


Figure 2.3. DOELAP Performance Test Results for the HSD Whole Body Dosimeter, Shallow Dose

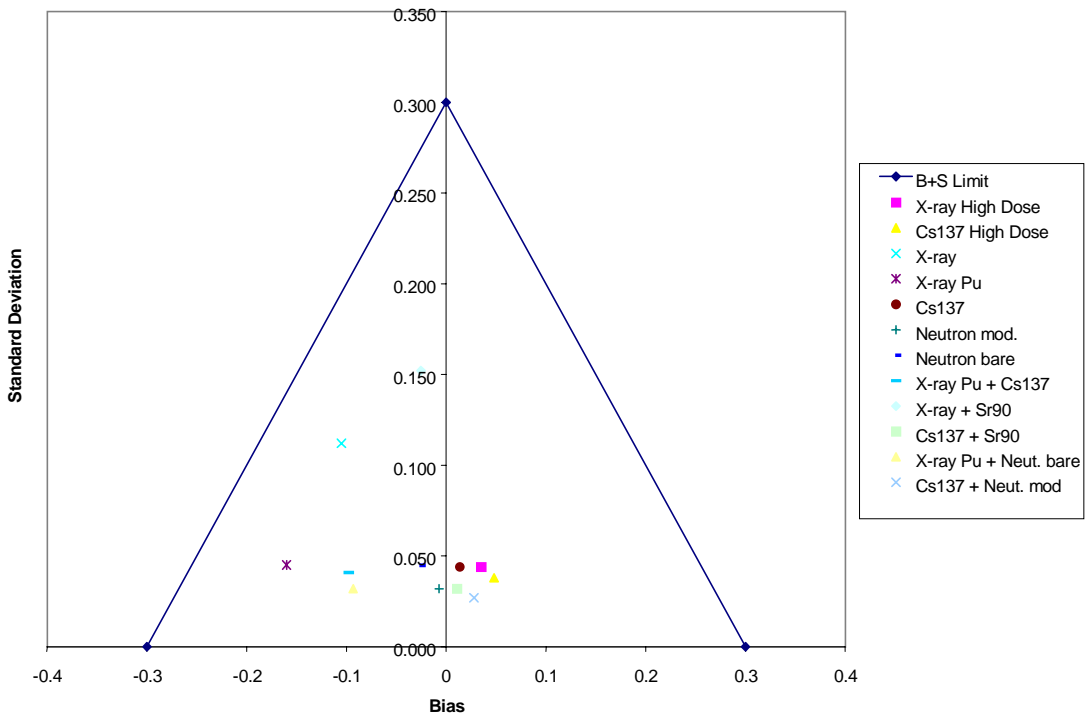


Figure 2.4. DOELAP Performance Test Results for the HCND Whole Body Dosimeter, Deep Dose

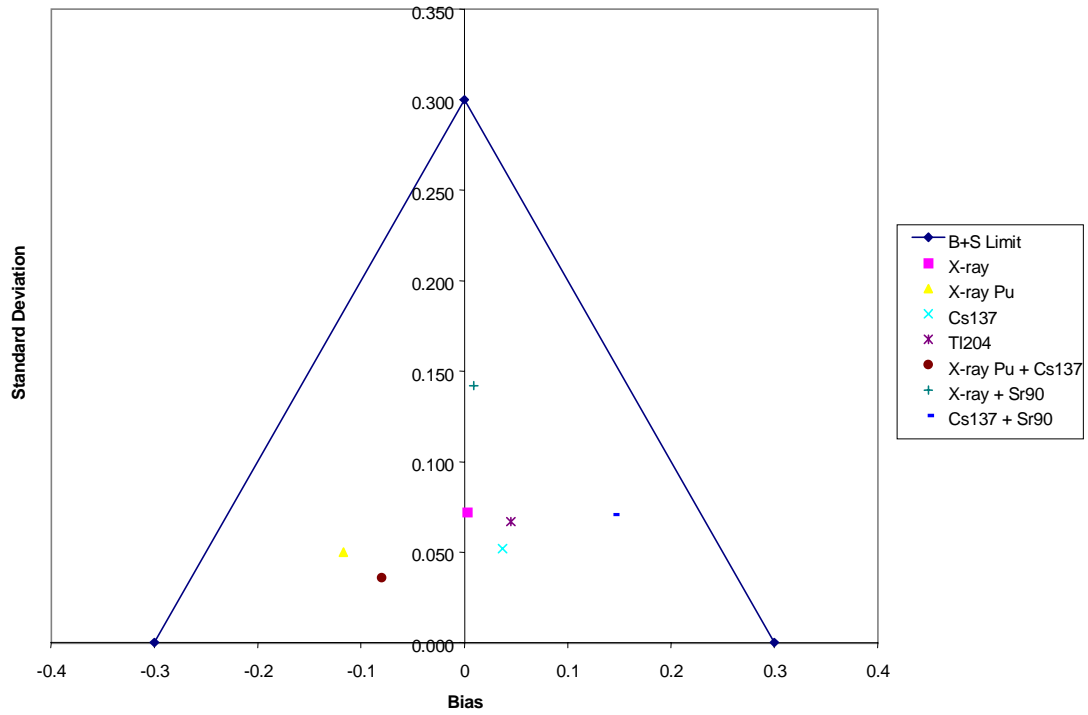


Figure 2.5. DOELAP Performance Test Results for the HCND Whole Body Dosimeter, Shallow Dose

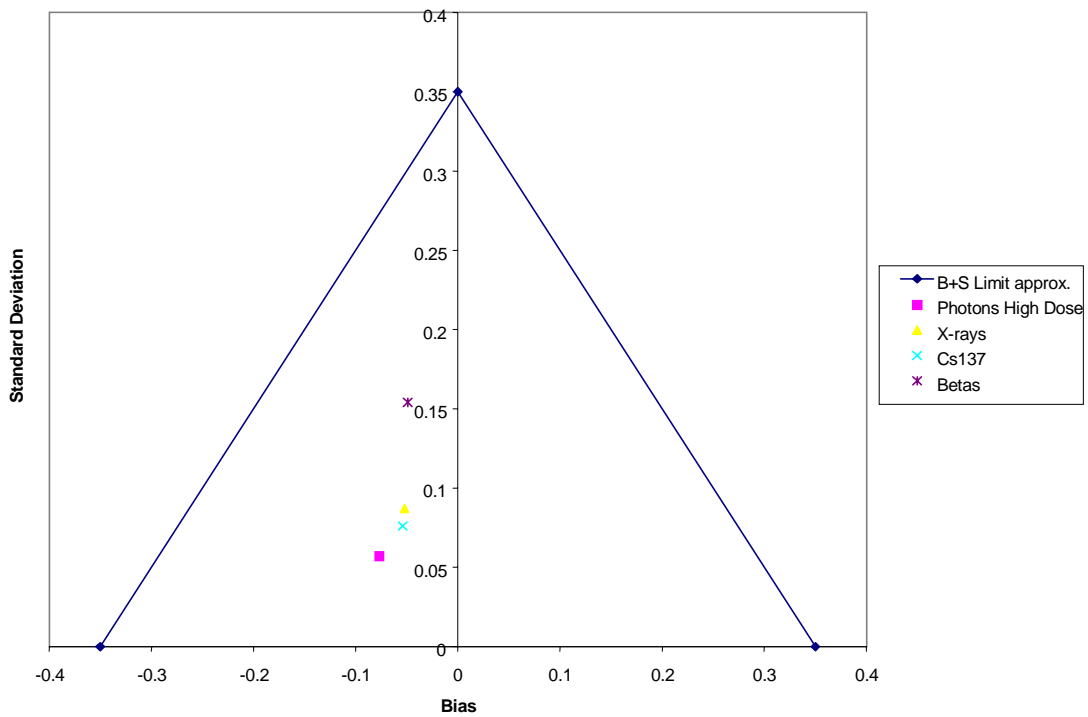


Figure 2.6. DOELAP Performance Test Results for the Hanford Ring Dosimeter, Shallow Dose

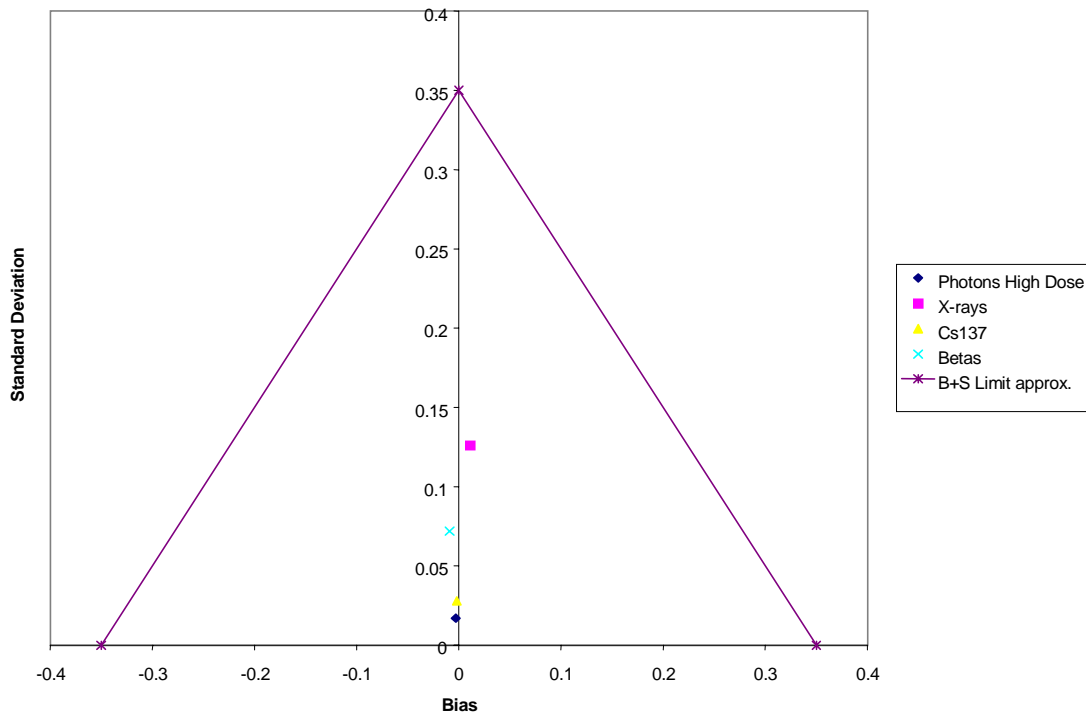


Figure 2.7. DOELAP Performance Test Results for the HSD Wrist Dosimeter, Shallow Dose

The onsite assessment was conducted from June 12 to 14, 2000 to examine HEDP documentation and practices relative to the requirements of the DOELAP Handbook (DOE 1986a). The assessment noted one deficiency and two concerns.^(a) The deficiency was for failure to consistently conduct maintenance on the TLD readers monthly as stated in HEDP procedures. The concerns were (paraphrased) as follows:

1. No acceptance criteria for the density thickness of finger rings.
2. A discrepancy between the technical basis manual and actual use of the algorithm concerning the zero dose value for finger rings.

Corrective actions on all three items were completed by the end of the calendar year.

2.3.4 National Voluntary Laboratory Accreditation Program

Performance testing and an onsite inspection occur approximately every 2 years for the NVLAP, which is operated by the NIST. Performance testing was conducted at the end of 1999, and the results were presented in last year's annual report (Lynch et al. 2000); but the onsite inspection did not occur until April 11 to 13, 2000. The onsite inspection examined HEDP documentation and practices relative to the requirements of the NIST Handbook 150-4 (NIST 1994). There was one finding citing the lack of a

(a) Deficiencies are issues that require immediate corrective actions and can preclude obtaining accreditation, and concerns are issues that require a formal corrective action plan.

procedure for redetermining the element correction coefficient for chipstrate TLDs (in finger rings). (The need for the procedure in our program had not occurred yet.) That procedure was written by July, and accreditation was granted in September.

2.3.5 Energy Northwest Assessment

From February 9 to 11, Energy Northwest, for which HEDP processes environmental dosimeters, audited our dosimetry practices against ANSI N545 (ANSI 1975), various Nuclear Regulatory Commission regulatory guides, and our own Quality Assurance (QA) Plan, technical basis manual, and procedures. No findings required a response; a few recommendations were quickly and easily implemented.

2.3.6 Self-Assessments

Self- (or internal) assessments of the HEDP are conducted annually. The 2000 self-assessment was conducted in May and focused on the status of corrective actions from previous assessments by various groups in preparation for the DOELAP onsite assessment (see Section 2.3.3).

In addition, the DOELAP deficiency mentioned in Section 2.3.3 was presented to PNNL's Price Anderson Act Amendment (PAAA) Working Group. The Working Group concluded that the deficiency constituted a reportable event and requested that a root cause analysis of the program be performed as part of the corrective actions. That root cause analysis was conducted in August and September, and it resulted in the following additional corrective actions:

- implementation of a schedule for periodic (at least four per year) surveillances by the program's quality engineer
- improvements in the process for changing procedures
- a review of all procedures to enhance tracking methods for steps that have definitive time constraints
- discussion among procedure authors concerning overspecifying steps in procedures that unnecessarily inhibit flexibility.

2.3.7 Environmental Dosimeter Intercomparison

HEDP participated in the 12th international environmental dosimeter intercomparison hosted by the Environmental Measurements Laboratory. At year-end, HEDP had analyzed the test dosimeters, but results of the intercomparison were still pending from the Environmental Measurements Laboratory.

2.4 Supporting Technical Studies

Seven technical studies or tasks were undertaken during 2000, as described in the following sections.

2.4.1 New External Dosimetry Code

HEDP began work on a new code that will operate on the Sun Enterprise computer that houses REX. The code, given the moniker Edipus, will be an Oracle relational database that will replace the series of codes presently operating on the VAX cluster. In 2000, the entity-relationship diagram was developed and work started on the coding.

2.4.2 Evaluation of Lead Impurity in Tin Filters in the 8825 Holders

As part of special testing of tin filters over TLD chip 4 in the 8825 holders (see Section 2.2.5), lead impurity was discovered in some tin filters. Additional testing indicated that lead was present in about 90% of the tin filters ranging from 2 to 4% (weight %). DOELAP and NVLAP test dosimeters were found to have essentially the same makeup of lead contamination as worker dosimeters so all DOELAP and NVLAP performance testing over the years was considered valid for the entire stock of holders. Irradiation tests on leaded versus unleaded filters for photons from 17 to 662 keV indicated that there are essentially no differences in doses calculated with the two groups. Therefore, a decision was made to not remove leaded filters from service.

2.4.3 Uncertainty Analyses

Analyses of overall uncertainty in the processing (in general, not of individual dosimeters) were conducted over the last 2 years for the 8825, 8816, CR39, and finger ring dosimeters. Uncertainties, at the 95% confidence level, for the 8825 HSD and 8825 portion of the HCND, were determined to be about 30% for the shallow, eye, and deep dose from photons and 60% for the deep dose from neutrons. The uncertainty in the 8816 deep dose from neutrons was about 12%. For neutron deep dose measured using CR39, the calculated uncertainty was about 23%. The uncertainties for the finger ring varied depending on the energy of the beta radiation, but for all beta radiations tested the uncertainties were less than 25%.

2.4.4 Effect of Lead Aprons on Response of 8825 and 8816 Dosimeters

To support a feasibility study on the use of lead aprons at the PFP, HEDP measured the change in response of the 8825 portion of the HCND 8825 (7777) to photons and the response of the 8816 portion of the HCND to neutrons. Photon response was measured for 17-, 59-, and 662-keV photons; and neutron response was measured for both moderated and unmoderated ²⁵²Cf neutrons. The impacts were evaluated for dosimeters worn on top of and underneath the lead aprons being evaluated.

The study concluded the following:

- For the 8825 dosimeter worn on top of the lead apron, the dosimeter will underestimate dose to unshielded portions of the body by about 35% for 59-keV photons and will be reasonably accurate for 17- and 662-keV photons. The dosimeter will overestimate dose to shielded portions of the body from both 17- and 59-keV photons and will be reasonably accurate for 662-keV photons.

- For the 8825 dosimeter worn underneath the lead apron, the dosimeter will be reasonably accurate for body parts under the apron regardless of photon energy. The dosimeter will significantly underestimate dose to unshielded parts of the body for 17- and 59-keV photons.
- Overall the lead apron reduced the shallow and deep dose from photons by about 100 fold for 17-keV photons, about 10 fold for 59-keV photons, and essentially 1 fold (no reduction) for 662-keV photons.
- For the 8816 dosimeter worn on top of the lead apron, there was essentially no impact on the neutron measurements for either the moderated or unmoderated neutrons.
- For the 8816 dosimeter worn under the lead apron, the dosimeter overestimated the neutron dose from unmoderated neutrons by 35% and underestimated the neutron dose from moderated neutrons by 25%.

Based on the study, a recommendation was made to wear an HCND under the apron and an 8825 (7777) dosimeter outside the apron.

2.4.5 Analysis of Phosphorus-32 in Sulfur Pellets and Hair

A special test was conducted to exercise the capability of PNNL's Radiological Chemistry Group to analyze ^{32}P in sulfur pellets from nuclear accident dosimeters and in human hair. Phosphorus-32 results from neutron activation of ^{32}S . The procedure to analyze these matrices for ^{32}P had not been tested for many years. Six sulfur pellets and six hair samples were spiked with various known amounts of ^{32}P and submitted along with three blank samples of each matrix. The laboratory provided acceptable results on all the samples.

2.4.6 Shallow Dose Rate from T-Handle Waste Sample Carriers

HEDP assisted the radiological control group at the 222-S Building studying the dose rate to extremities for workers carrying vials of waste tank samples in T-handle carriers. Holes in the top of the leaded carriers produce collimated beams of gamma and beta radiation upward toward the hands. In use, the dose rate at the hands is surveyed using an RO-3 or RO-20 ionization chamber survey instrument. However, because the beam diameter is smaller than the ionization chamber diameter, correction factors need to be applied to the ionization chamber readings. Chipstrate arrays were used to determine the size and shape of the beam and the correction factors for the RO-3 and RO-20 survey instruments. HSDs taped to cardboard sheets were also used to determine beta energy adjustment factors needed to properly interpret the readings on the chipstrates. These measurements were performed for different types of waste samples (solids or liquids) and different sample volumes.

2.5 Skin Contaminations

Hanford skin contamination statistics are provided in Table 2.5. These statistics were first included in this report in 1999, and the number of skin contaminations decreased significantly in 2000. The reason for this was not determined, although it certainly was not related to the amount of work being performed in contaminated areas.

Table 2.5. Number of Skin Contaminations (Worker-Events)^(a)

Contractor	Number of Contaminations	
	1999	2000
PHMC ^(b)	39	NA ^(c)
FH	NA	10
CHG	NA	7
PNNL	18	1
ERC	0	Not Provided
DOE	0	0
Total	57	18
(a) Each contamination event for a single worker counted separately.		
(b) PHMC included both FH and CHG in 1999.		
(c) NA = not applicable.		

2.6 Program-Related Professional Activities

Staff activities, presentations, publications, and professional memberships during 2000 are listed in this section.

2.6.1 Activities

Jack J. Fix was involved in several professional external dosimetry activities, outside of the Hanford Site. He participated

- in DOELAP Oversight Board meetings from March 7 to 9, 2000 and August 14 to 16, 2000.
- as the lead DOELAP assessor of the Y-12 dosimetry program from January 26 to 28, 2000.
- as the manager of Battelle project to add participating U.S. Commercial Nuclear Power Plant workers to the International Agency for Research on Cancer (IARC) Collaborative Study involving workers from 17 countries. This study also includes Hanford workers.

- as principal investigator in a National Institute of Occupational Safety and Health (NIOSH) project concerning U.S. participants in the IARC study.
- as principal investigator to develop a DOE central dose repository and to include dose parameters in the DOE Epidemiologic Surveillance Program.

Bruce A. Rathbone was similarly involved in professional external dosimetry activities, outside of the Hanford Site, and participated

- as DOELAP assessor of the Oak Ridge National Laboratory dosimetry program from January 10 to 11, 2000.
- as DOELAP assessor of the Lawrence Livermore National Laboratory dosimetry program from July 18 to 19, 2000.

2.6.2 Presentations

Huneycutt, S. E., “Eddy Current Methods for Acceptance Testing TLD Holders,” PNNL-SA-33635, September 20, 2000, Harshaw TLD User’s Group Symposium, Herndon, Virginia.

Rathbone, B. A., “Experiences in ANSI N13.29 Pilot Testing Using the Harshaw 8807 Environmental Dosimeter.” PNNL-SA-33640, September 20, 2000, Harshaw TLD User’s Group Symposium, Herndon, Virginia.

2.6.3 Publications

Scherpelz, R. I., J. J. Fix, and B. A. Rathbone. 2000. *Validation of Hanford Personnel and Extremity Dosimeters in Plutonium Environments*. PNNL-13136, Pacific Northwest National Laboratory, Richland, Washington.

2.6.4 Professional Memberships

Fix, J. J., Member of DOELAP Oversight Board.

Fix, J. J., Chair of Health Physics Society Standards Committee.

Fix, J. J., Consultant to ANSI N13.29, *American National Standard for Dosimetry - Environmental Dosimetry Performance Criteria for Testing*, and N13.37, *American National Standard for Dosimetry, Performance Testing, and Procedural Specifications for Environmental Thermoluminescent Dosimetry*, working groups.

Rathbone, B. A., Member, HPS Working Group for ANSI N13.37, *American National Standard for Environmental Dosimeters*.

3.0 Hanford Internal Dosimetry Program

The Hanford Internal Dosimetry Program (HIDP) was initiated in 1946 to provide for the assessment and documentation of occupational doses from intakes of radionuclides at the Hanford Site. The program is administered in support of Hanford radiation protection programs, as required by 10 CFR 835, *Occupational Radiation Protection*. Additional guidance is provided by the implementation guide (DOE 1999a) and the technical standard (DOE 1999b). The program provides the following internal dosimetry services:

- administration of a routine excreta monitoring program
- investigation and assessment of potential intakes
- monitoring performance of the contract excreta bioassay laboratory
- selection and application of models, procedures, and practices for evaluating intakes
- technical support to RL, DOE-Office of River Protection (ORP), and to Hanford Site contractors
- 24-hour, single-point-of-contact technical support for radiological incidents at Hanford
- bioassay scheduling for the Fluor Hanford companies, CHG, DOE-ORP, and RL.

3.1 Routine Operations

Operational details of the HIDP are described in the following documents:

- The technical aspects of internal dose calculations are established in *Methods and Models of the Hanford Internal Dosimetry Program*,^(a) which replaced the *Technical Basis for Internal Dosimetry at Hanford*, Rev. 1 (Sula, Carbaugh, and Bihl 1991) in CY 2000.
- The protocols and practices for operation of the program and coordination with the Hanford Site contractors are established in the *Hanford Internal Dosimetry Program Manual*.^(b)

(a) Pacific Northwest National Laboratory. Current version. *Hanford Internal Dosimetry Technical Basis Manual*. PNNL-MA-860, Richland, Washington. (Internal manual.). Available URL: <http://www.pnl.gov/eshs/pub/pnnl860.html>

(b) Pacific Northwest National Laboratory. Current version. *Hanford Internal Dosimetry Program Manual*. PNL-MA-552, Rev. 3, Richland, Washington. (Internal manual.) Available URL: <http://www.pnl.gov/eshs/pub/pnl552.html>

- Detailed procedures are contained in the *Hanford Internal Dosimetry Procedures Manual*.^(a)
- Protocols for responding to radiological incidents are contained in the *On-Call Exposure Evaluator Manual*.^(b)
- Quality assurance for the program is covered in the Quality Assurance Plan for the Operation of the *Hanford Internal Dosimetry Program*.^(c)
- The technical agreements with the excreta lab are established by a contractual Statement of Work (SOW).

The practices and technical aspects of operating the In Vivo Monitoring Program for Hanford are established in the *In Vivo Monitoring Program Manual*^(d) (see Chapter 4.0). Individual assessments of internal dose are documented in each individual's file in the Hanford Radiation Records Program files. Bioassay measurement results and internal doses are maintained in the REX database, which is operated by the Hanford Radiation Records Program (see Chapter 5.0).

Intakes of radionuclides are generally prevented by containment or other protective measures; therefore, intakes are normally assumed to result from an acute intake. Dose assessment is based on this assumption, except for work with tritium, for which chronic or intermittent acute intakes may be assumed. Four cases of intermittent tritium intakes were tracked throughout the year and assessed at the end of the year.

Needs testing for bioassay requirements and waiving of the routine bioassay if a worker did not enter an area requiring specific bioassays was resumed for FH, CHG, and DOE workers in March 2000.

3.1.1 Bioassay Capabilities

Bioassay monitoring is performed regularly for workers who might inhale, ingest, or absorb radionuclides into their bodies in the course of their jobs. Measurement types and frequencies are based on the radionuclides of concern, their anticipated physical and chemical form, the relative risks of intakes for workers, and the costs of the bioassay (both analysis cost and cost of the worker's time away from the job). Minimum detectable activities (MDAs) and screening levels for routine excreta and in vivo bioassay measurements are shown in Tables 3.1 and 3.2. MDAs for emergency and expedited excreta measurements are provided in Table 3.3.

-
- (a) Pacific Northwest National Laboratory. Current version. *Hanford Internal Dosimetry Procedures Manual*. PNL-MA-565, Richland, Washington. (Internal manual.)
- (b) Pacific Northwest National Laboratory. Current version. *On-Call Exposure Evaluator Manual*. PNL-MA-857, Richland, Washington. (Internal manual.)
- (c) Pacific Northwest National Laboratory. Current version. *Quality Assurance Plan for the Operation of the Hanford Internal Dosimetry Program*. LSC-026, Richland, Washington. (Internal manual.)
- (d) Pacific Northwest National Laboratory. Current version. *In Vivo Monitoring Program Manual*. PNL-MA-574, Richland, Washington. (Internal manual.)

Table 3.1. Specified Minimum Detectable Activities and Screening Levels
for Routine Excreta Analyses During CY 2000

Analysis ^(a)	Contractual MDA ^(b,c)	Screening Level And Sampling Frequency ^(c,d)
²³⁸ Pu, ²³⁹ Pu	0.02 dpm	0.01 dpm ^(e) (A)
²³⁸ Pu, ²³⁹ Pu (IPUL)	0.005 dpm	0.003 dpm ^(e) (A)
⁹⁰ Sr	10 dpm	5 dpm (A) 5 dpm (BE)
²³⁴ U, ^(f) ²³⁸ U	0.02 dpm	0.15 dpm ^(g) (A,Q)
²³⁵ U	0.02 dpm	0.01 dpm ^(e) (A, Q)
²⁴¹ Am, ²⁴³ Am, ²⁴² Cm	0.02 dpm	0.01 dpm ^(e) (A)
²²⁸ Th, ²²⁹ Th, ²³² Th	0.10 dpm	0.05 dpm (not established)
²²⁵ Ac, ²²⁷ Th	0.10 dpm	0.05 dpm (not established)
Elemental U	0.06 µg	0.2 µg ^(g) (Q)
Tritium	20 dpm/ml	80 dpm/ml ^(h) (M)
<p>(a) Analysis of urine samples, unless otherwise indicated.</p> <p>(b) Specified MDA based on Type I and Type II errors of no greater than 5%, as described in the SOW (a copy is available in the Hanford Radiation Protection Historical Files).</p> <p>(c) Amount per total sample volume, unless otherwise indicated.</p> <p>(d) Follow-up actions are taken when this value is exceeded (routine bioassay monitoring frequency: A - annual, BE - biennial, M - monthly, Q - quarterly).</p> <p>(e) Screening level is anything detected. The detection decision level varies from sample to sample. Value listed is nominal.</p> <p>(f) The lab cannot discriminate between ²³³U and ²³⁴U and reports the results as ²³⁴U (beginning in 1994).</p> <p>(g) Upper level of expected environmentally derived uranium in urine for the Hanford region.</p> <p>(h) Special screening levels are established for short-term tritium work where beginning and ending work samples are obtained instead of monthly routine sampling.</p>		

The excreta analyses parameters listed in Tables 3.1 and 3.3 were unchanged from 1999.

3.1.2 Excreta Bioassay Contract Activities

Severn Trent Laboratories (STL) purchased Quanterra Environmental Services in 2000, and the bioassay analytical contract was novated to the new company. Facilities and personnel remained unchanged.

Two major problems were tracked during the year: an extensive sample backlog of alpha spectrometry samples and excessive ²⁴³Am false positive results. The backlog developed late in 1999, and was attributed by the contractor to difficulty in hiring and retaining staff, and to a large influx of samples from non-Hanford clients. STL first responded by assigning extra personnel for chemical separations, but the ultimate fix required purchase of additional instrumentation. Average turn-around times were back to normal by the middle of summer. The ²⁴³Am problem appeared to be due to the lack of reagent blank data for this procedure. Although the contract requires reagent blank subtraction for all results, the required data were not available for this relatively new and minimally used procedure until late in the year. Reagent blank subtraction is expected to correct the false positive problem.

Table 3.2. Minimum Detectable Activities and Screening Levels
for Routine In Vivo Measurements During CY 2000

Measurement/Radionuclide ^(a)	MDA ^(b) (nCi)	Screening Level ^(c) (nCi)
Standup Whole Body Count		
⁶⁰ Co	1.25	4
¹⁵⁴ Eu	3.75	Any detected
¹³⁷ Cs	1.30	Any detected
Coaxial Germanium Whole Body Count		
¹³⁷ Cs	0.80	Any detected
Lung Count		
²³⁵ U	0.09	Any detected
²³⁸ U (by ²³⁴ Th)	1.5	Any detected
²⁴¹ Am	0.16	Any detected
(a) For selected radionuclides. (The detection of radionuclides not listed resulted in follow-up, except for ²¹⁴ Bi.) (b) For each in vivo count, the decision levels (approximately half of the MDAs) were reported under the heading “detection limit” to REX, but, in terms of overall detectability for all measurements, the above MDAs were still applicable. (c) Level for which an investigation of internal exposure was considered. Any detected activity above background (i.e., above the decision level) was reported to the HIDP.		

3.1.3 Excreta Bioassay Monitoring Activities

Sample requests can be categorized as standard or nonstandard. Standard requests are those generated by the REX database from a predetermined, routine schedule (e.g., a worker may be scheduled for an annual sample collected every April). These requests are downloaded from REX and electronically transferred to the analysis laboratory just before the start of each month. All other requests are considered nonstandard requests. Contractors and HIDP staff manually enter the nonstandard requests into REX. HIDP staff check the nonstandard request file in REX for input errors and perform the electronic transfer of the requests to the laboratory. Figure 3.1 shows the monthly distribution of standard and nonstandard requests for 2000. A total of 4,685 samples were requested in 2000, down 2% from the 1999 requests. The number of standard requests (53%) slightly exceeded the number of nonstandard requests. Overall, the totals were not significantly different from 1999.

During 2000, 5,369 excreta bioassay measurements were successfully performed in support of Hanford activities, excluding cancellations, no-samples, samples without valid results, and QC samples (isotopic results for each element count as one measurement). Of these, 95% were classified as routine (including measurements on visitors) and 5% were due to special circumstances, such as response to unplanned potential intakes or followup analyses to high routine measurements. These percentages of routine and special measurements were virtually identical to those of 1999.

Table 3.3. Specified Minimum Detectable Activities for Emergency and Expedited Excreta Bioassay During CY 2000

Analysis ^(a)	MDA (Per Sample)	
	Urine	Feces
Emergency Analyses ^(b)		
Isotopic Plutonium by Alpha Spectrometry	0.5 dpm	9 dpm
Isotopic Uranium by Alpha Spectrometry	1.0 dpm	12 dpm
²⁴¹ Am by Alpha Spectrometry	1.0 dpm	20 dpm
²⁴¹ Am by LEPD ^(c)	20 dpm	20 dpm
Total Radiostrontium	80 dpm	450 dpm
Elemental Uranium	7 µg	8 µg
Tritium	100 dpm/ml	NA ^(e)
Expedited Analyses ^(d)		
Isotopic Plutonium by Alpha Spectrometry	0.08 dpm	3 dpm
Isotopic Uranium by Alpha Spectrometry	0.12 dpm	4 dpm
²⁴¹ Am by Alpha Spectrometry	0.08 dpm	6 dpm
²⁴¹ Am by LEPD	5 dpm	5 dpm
Total Radiostrontium	50 dpm	150 dpm
Elemental Uranium	0.5 µg	5 µg
Tritium	100 dpm/ml	NA
(a) For the more critical analyses only. The list does not contain all of the analyses covered in the contract. (b) Verbal reporting time was generally within 8 hours after receipt of the sample; reporting times were even shorter for some analyses. (c) LEPD = low-energy photon detector; direct counting of X-rays without radiochemical separation. (d) Verbal reporting time was by 9:00 a.m. on the second business day after receipt of the sample. (e) NA = not applicable.		

Figure 3.2 shows the trend in routine urinalyses since 1994. The figure shows that the number of routine measurements in 2000 was the highest in the last 5 years, up about 14% from 1999, but generally similar to 1998 and 1999. Increases occurred in all nuclide categories except “other.” Routine analyses in 1998 through 2000 exceed the numbers in 1995 and 1996, reflecting primarily increased work in contaminated areas. The large decrease between 1994 and 1995 to 1996 demonstrates the results of major efforts to tighten the requirements for placing workers on routine bioassay schedules and to remove from routine schedules workers who were at negligible risk for intakes.

Details on the type of excreta measurements categorized by contractor are provided in Table 3.4. Overall, the number of excreta measurements increased about 11% from 1999, with the largest increase in ⁹⁰Sr analyses. The percentages of excreta measurements for the three major contractors remained about the same.

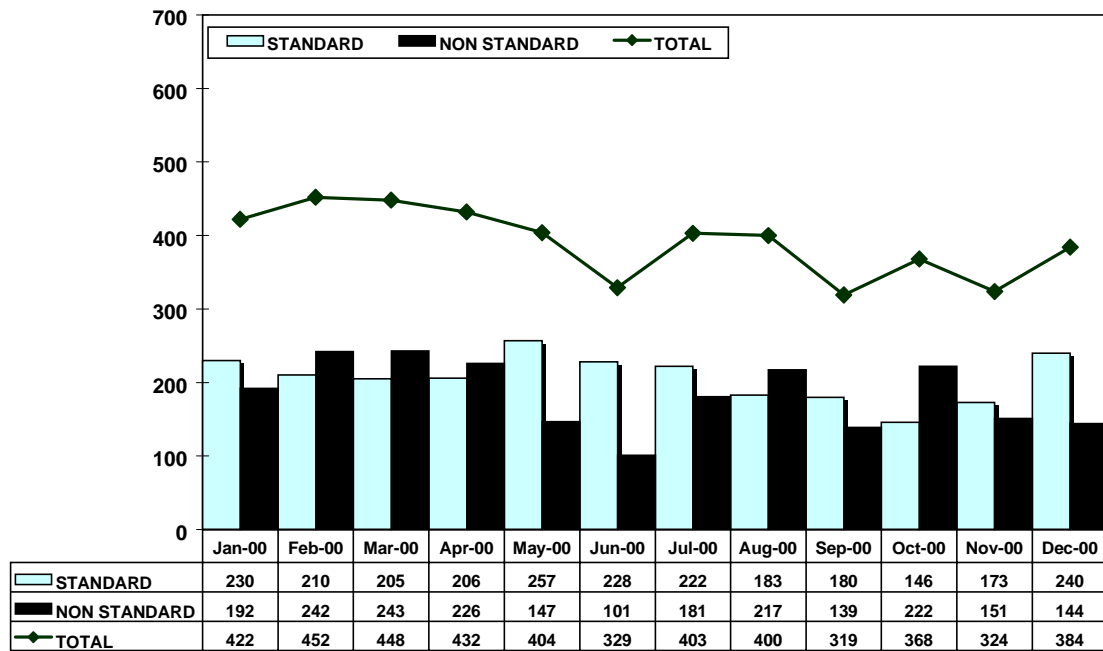


Figure 3.1. Standard and Nonstandard Excreta Requests by Month for 2000

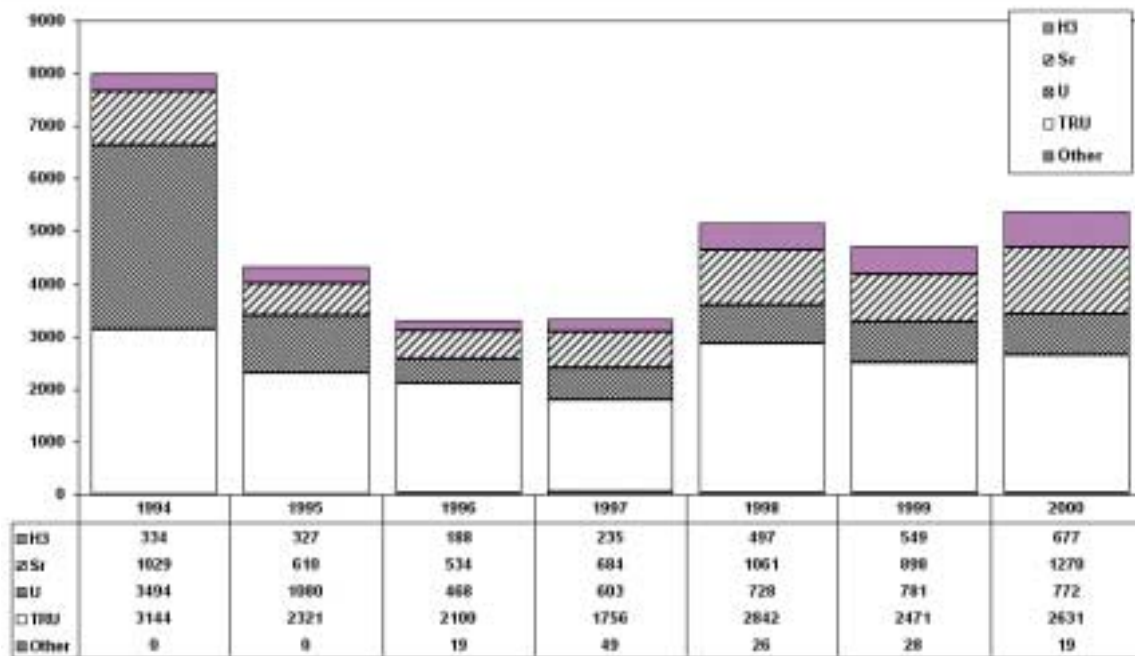


Figure 3.2. Routine Urine Measurements Made from 1994 Through 2000

Table 3.4. Worker Excreta Measurements Reported in 2000

Type/Reason	DOE	PNNL	BHI	FH	CHG	Other	Total
³ H- urine							
Routine schedule	0	674	0	2	0	0	676
Special request	0	1	0	0	0	0	1
⁹⁰ Sr - urine							
Routine schedule	81	226	284	442	170	1	1,204
Special request	1	1	2	26	35	1	66
Uranium - urine							
Routine schedule	21	407	147	153	6	0	734
Special request	0	23	4	11	0	0	38
Plutonium - urine							
Routine schedule	58	295	381	1,224	158	1	2,117
Special request	0	23	7	35	7	1	73
Other - urine							
Routine schedule	1	202	0	119	3	0	325
Special request	0	31	4	1	0	0	36
TRU - fecal							
Routine schedule	0	1	16	4	0	0	21
Special request	0	37	8	32	1	0	78
Analysis Totals	162	1,921	853	2,049	380	4	5,369

Not all excreta bioassay requests produce valid measurement results; these are referred to as “no-samples.” When a sample is not obtained, it has to be requested again. (The following statistics refer to the number of unsuccessful attempts to obtain a sample within the 10-day window specified in the SOW with the laboratory; statistics in the next paragraph address the question as to whether or not a sample was eventually collected). In 2000, 611 excreta sample requests were designated as no-samples, compared with 697 no-samples in 1999. In terms of percentage of total requests, the 2000 rate (11%) was somewhat less than previous years (15%, 18%, and 21% in 1999, 1998, and 1997, respectively). In addition there were 136 canceled requests that also show in the records. Unsuccessful sample collections (their associated no-sample code and percentage of the total no-samples) were attributed to the following causes: kit not delivered (ND, 6%), no sample received (NS, 23%), lost container (LC, 25%), insufficient sample volume (IS, 24%), and failed analyses (FA, 22%). The percentage of each type of unsuccessful sample is similar to previous years except for fewer lost containers and an increase in the insufficient sample volume category. The number of failed analyses was similar to the previous 2 years’ rates; however, those rates are considerably above the historical average.

There is special interest in whether or not bioassay samples are ultimately (i.e., after several attempts) collected within the grace period. Figure 3.3 shows the number of excreta bioassay samples not collected within the grace period. The 58 samples not collected in the grace period represent about 1% of the total samples obtained. The statistics for 2000 are about twice as high as they were for 1999. In large part, this is due to the fact that the grace period concept was first implemented in 1999 and the total of 25 samples

not collected within the grace period that year only covered the half-year following its implementation. The statistics do not include situations where collecting a sample was not considered reasonable, such as during pregnancy leave, short- or long-term disability leave, or a long-term work assignment at another location. Figure 3.4 shows a similar statistic for samples requested from terminating workers, i.e., samples not ultimately collected.

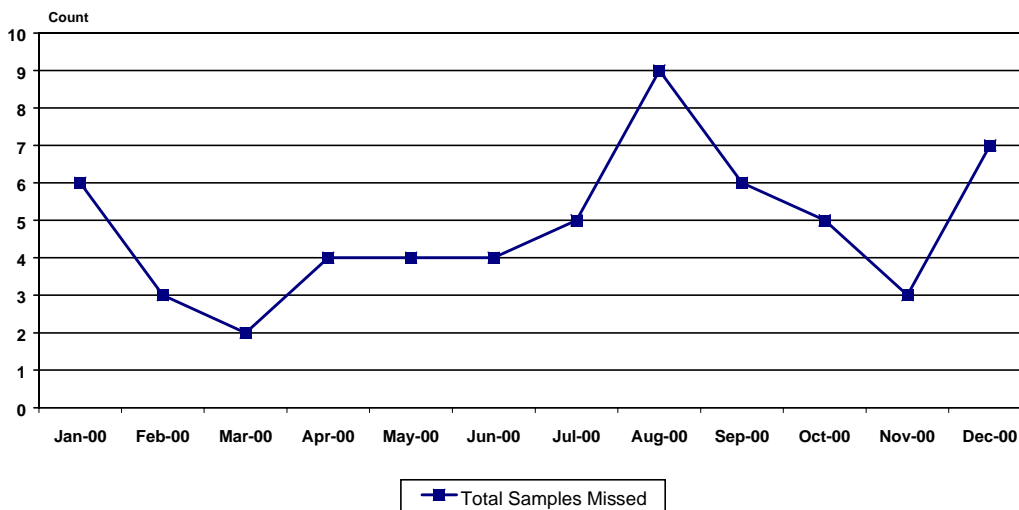


Figure 3.3. Excreta Samples Not Obtained in the Grace Period

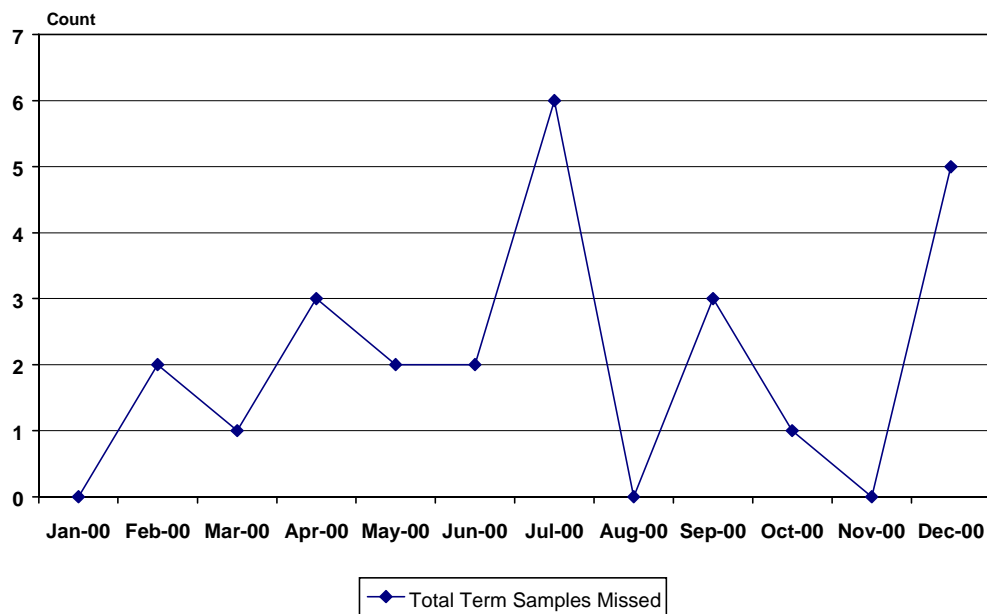


Figure 3.4. Termination Excreta Samples Not Obtained

3.1.4 Potential Intake Evaluations

Investigations of possible radionuclide intakes are performed following an indication from a routinely scheduled bioassay measurement (high routine) or for a potential exposure incident identified in the workplace (incident). Potential exposure incidents are identified by workplace indicators such as air sampling, contamination surveys, nasal smears, or smears from potentially contaminated wounds. Evaluations are also performed for newly hired workers who incur intakes prior to their Hanford employment to ensure that the pre-Hanford intake information is converted to dose in a manner consistent with DOE regulations. Reevaluations of internal dose may also be conducted for workers with significant long-term body burdens.

During 2000, 21 incidents with the potential for intake, involving 65 workers, were identified through workplace monitoring. Of the 65 workers involved in the incidents, intakes were confirmed for 33 workers, those coming from 15 of the incidents. The highest calculated dose among the 33 workers was an 80-mrem committed effective dose equivalent (CEDE). Table 3.5 shows the incident breakdown by contractor, facility, and principal radionuclides.

In addition to incidents, potential intakes can be discovered through the routine bioassay program, although in recent years very few actual (i.e., confirmed) intakes have been discovered this way. In 2000, 103 evaluations were started because of routine bioassay results that exceeded the criteria for investigation (excluding evaluations started because of intakes incurred prior to employment at Hanford). Intakes were assigned for six workers. Four of those workers had intermittent exposure to tritium, which was treated as chronic intake. The highest internal dose revealed through the routine bioassay program was a 2-mrem CEDE. Table 3.6 shows internal dose evaluations for 2000 resulting from high routine bioassay results. Table 3.7 indicates the trends in all types of potential intake evaluations since 1994.

Table 3.5. Summary of Potential Intake Incidents During 2000

Area	Facility	Custodian	Number of Incidents	Number of Workers	Worker Contractor	Principal Radionuclides
100-K	105-KE	BHI	1	1	BHI	¹³⁷ Cs, ⁹⁰ Sr
200-E	204-AR	CHG	1	3	CHG	¹³⁷ Cs, ⁹⁰ Sr
200-E	241-A	CHG	1	7 5	CHG FH	¹³⁷ Cs, ⁹⁰ Sr
200-E	244-AR	CHG	1	5	CHG	¹³⁷ Cs, ⁹⁰ Sr, Pu-mix
200-W	233-S	BHI	7	9	BHI	Pu-mix
200-W	234-5Z	FH	1	3	FH	Pu-mix
200-W	241-S	CHG	1	5	CHG	¹³⁷ Cs, ⁹⁰ Sr
200-W	AN-103	CHG	1	1	CHG	¹³⁷ Cs
300	324	FH	2	3	FH	¹³⁷ Cs, ⁹⁰ Sr
300	325	PNNL	3	11	PNNL	Pu-mix
300	327	FH	2	12	FH	¹³⁷ Cs, ²⁴¹ Am, Pu
Total			21	65		

Table 3.6. Summary of Intake Cases Identified Through the Routine Bioassay Program During 2000

Area	Building	Custodian	Number of Workers	Contractor	Principal Nuclide
200-E	Tank Farms	CHG	1	CHG	¹³⁷ Cs
200-W	221-T	FH	1	FH	⁹⁹ Tc, ¹³⁷ Cs
300	325	PNNL	4	PNNL	³ H ^(a)
Total			6		
(a) All cases were treated as chronic intakes; i.e., one dose evaluation each at the end of the year.					

Table 3.7. Comparison of Potential Intakes by Reason Code, 1994 to 2000

	1994	1995	1996	1997	1998	1999	2000
Incident, Total	33	51	42	51	186	57	65
Confirmed	7	12	11	12	8	15	33
Unconfirmed	26	39	30	33	178	42	32
Open			1	6		0	0
High Routine, Total	91	59	40	85	136	96	99
Confirmed	15	1	5	10	22	5	2
Unconfirmed	76	58	33	75	114	91	97
Open						0	0
Chronic Exposure, Total	0	0	0	2	0	12	4
Confirmed				2		12	4
Unconfirmed				0		0	0
Pre-Hanford, Total	35	9	12	10	13	24	37
Confirmed	31	9	11	10	9	23	37
Unconfirmed	4		1		4	1	0
Open							0
Totals	162	119	94	148	335	189	205
Confirmed	53	22	27	34	39	55	76
Unconfirmed	109	97	64	108	296	134	129
Open						0	0
Reevaluations Completed	8	17	1	0	3	0	0

Figure 3.5 shows the workload of open cases as recorded at the end of each month. This figure suggests that about 60 evaluations per month were in process during 2000.

The range of internal doses assigned to the Hanford work force in 2000 is summarized in Table 3.8. 2000 is the second (and consecutive) year since the start of tracking of these statistics that there was no assignment of internal dose exceeding a 100-mrem CEDE.

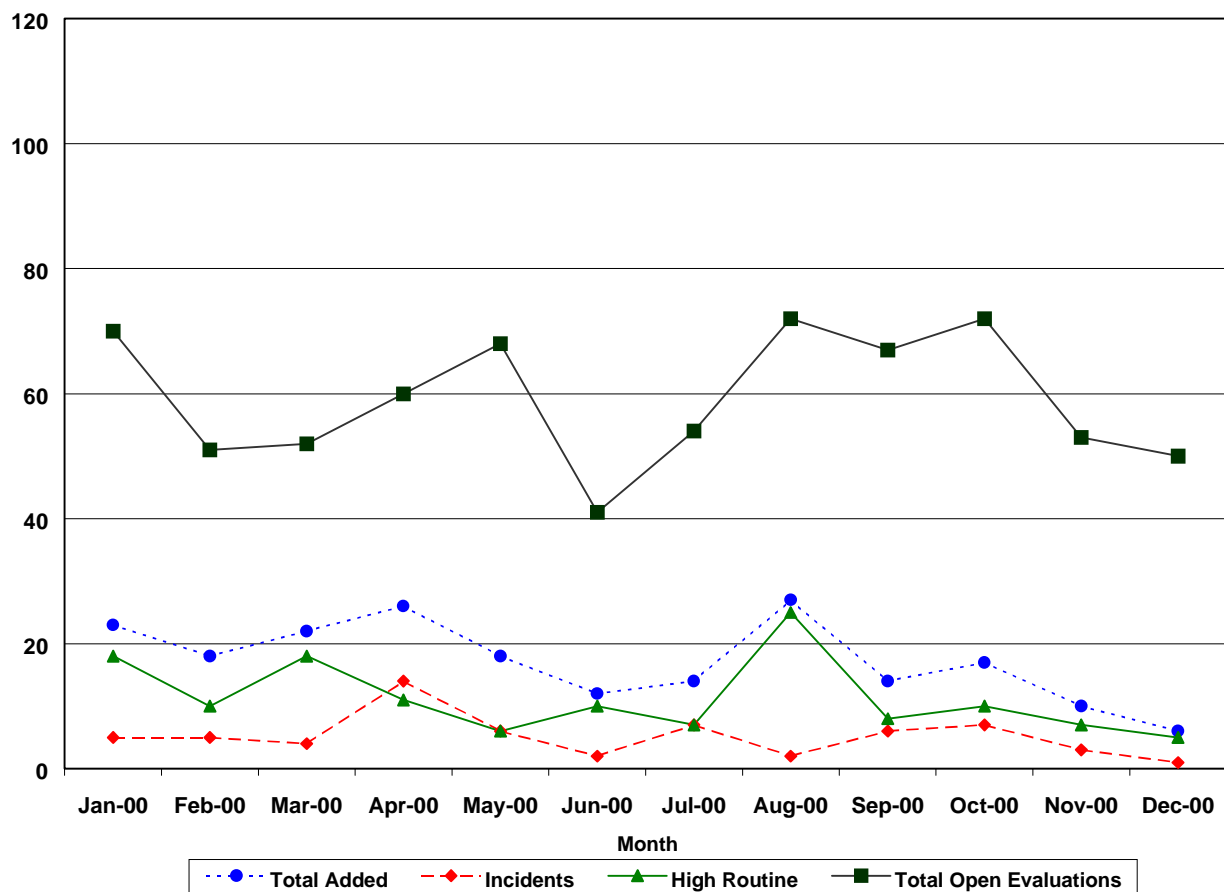


Figure 3.5. Number of Open Evaluations by Month. (Top curve shows number of evaluations open on the last day of each month.)

Table 3.8. Range of New Internal Doses Assigned to the Hanford Work Force in 2000

Dose (mrem) ^(a)	Number of Workers					
	DOE	FH	PNNL	BHI	CHG	Total
<100	0	16	13	7	3	39
100 - <500	0	0	0	0	0	0
500 - <2000	0	0	0	0	0	0
2000 - <5000	0	0	0	0	0	0
>5000	0	0	0	0	0	0
(a) CEDE, based on 2000 evaluations, although the intake could have occurred in any year; excludes reevaluations.						

3.2 Program Changes and Improvements

Three program changes and improvements were made during CY 2000 as described in the following sections.

3.2.1 Methods and Models Manual Issued

The internal manual, *Methods and Models of the Hanford Internal Dosimetry Program*, (PNNL-MA-860) was completed and issued in September 2000, both as a controlled hard-copy manual and as an online manual. This manual replaced the 1991 document, *Technical Basis for Internal Dosimetry at Hanford* (PNL-6866 Rev. 1) as the program's reference document detailing how bioassay data are interpreted and how internal dosimetry is performed at the Hanford Site. The former document has been retired.

The "M&M" manual specifies the biokinetic model used for each radioelement, along with the assumptions used in program design and data interpretation. Generally, the biokinetic models of Publication 30 of the International Commission on Radiological Protection (ICRP 1979) are used; however, some of the compartment fractions and biological half-times have been modified to approximate more recent ICRP models. The ICRP 30 respiratory tract model has been retained, however the default assumption for inhalation particle size was changed from 1- μm to 5- μm activity median aerodynamic diameter (AMAD), based on current recommendations of the ICRP and a literature review.

The manual also tabulates many values for intake retention, excretion, dose coefficients, minimum detectable doses for various bioassay intervals, and it provides some historical background on sources and past internal dosimetry practices at Hanford. Specific chapters of the manual are devoted to tritium, cesium, strontium, uranium, plutonium, americium, ^{60}Co and corrosion products, iodine, europium, and neptunium. Mixtures of cesium, strontium, and plutonium are addressed in an appendix.

The manual can be found as a pdf format file on the World Wide Web, at the following URL address: <http://www.pnl.gov/eshs/pub/pnnl860.html>

3.2.2 Changes to the Hanford Internal Dosimetry Program Manual

Changes to the program instituted through the *Hanford Internal Dosimetry Program Manual* are summarized in Table 3.9.

3.2.3 Update on New Decision Level for Alpha Spectrometry

The reasons for changing the computational method for determining the decision level (L_c) were reported in last year's annual report. The change was originally implemented using the following formula:

$$L_c = \overline{x_B} + 2.05 \bullet (\text{TPU})$$

Table 3.9. Changes to the *Hanford Internal Dosimetry Program Manual*

Section	Changes
Entire manual	References to the Hanford Internal Dosimetry Project were changed to the Hanford Internal Dosimetry Program to reflect the current program name.
Entire manual	References to the Hanford Site Radiological Control Manual (HSCRM) were removed and replaced with applicable guidances
Entire manual	References were added to the <i>Methods and Models of the Hanford Internal Dosimetry Program</i> , PNNL-MA-860, as a replacement manual for the document <i>Technical Basis for Internal Dosimetry at Hanford</i> , PNL-6866, Rev. 1.
6.0 Bioassay Services	Sections relevant to the excreta contract laboratory were updated to reflect the current contract specifications
6.0 Bioassay Services	Sections relevant to the In Vivo Monitoring Program were updated to reflect the capabilities of their new software analysis program (Abacos).
2.1.3 and 3.1.2	Wording changed to clarify goal of completing evaluations within 3 months of receiving all pertinent data.

where TPU is the total propagated uncertainty for the reported result. However, it was later realized that inclusion of the mean blank value ($\overline{x_B}$) in the equation was inappropriate, because the value was also subtracted from the reported result. The present equation specified in the contract SOW is as follows:

$$L_c = 2 \bullet (TPU)$$

In addition to removing the mean blank value, the fractional portion of the multiplier was dropped for simplicity.

3.3 Program Assessments

Six program assessments were conducted during 2000, as described in the following sections.

3.3.1 Excreta Quality Control Oversight Program

The excreta QC oversight program operated as usual throughout 2000; however, the Quality Control Report for the first operational year of the new contract (September 1999 through September 2000) was still being drafted at the end of the year. Preliminary results indicated that laboratory performance was consistent with previous years, but there were significant discrepancies between plutonium spike activities reported by the preparation laboratory and analytical results during June through August. However, the high plutonium blank and spike results were considered to be the result of problems in the spiking laboratory, and not with the analytical contractor. Routine worker samples and blank samples submitted to the analytical contractor without going through the prep lab did not show high results.

Although no source of the contamination in the prep lab was identified, minor modification to the addition technique and the prep area appear to have corrected the problem. The time sample containers are open is now minimized by pre-weighing added water and completing the task as quickly as possible. Blank samples are prepared in a laminar flow hood. Also, all reagent materials were replaced with new stock, and quartz-distilled water was used instead of just Nanopure^{TM(a)} water.

3.3.2 Onsite Inspection of the Excreta Contract Laboratory

The annual QA assessment of STL performance under Contract 313500 was conducted in November 2000. In addition to the contract's QA requirements, the audit base included the contractor's Quality Assurance Management Plan and procedures. Requirements not specifically evaluated during the Environmental Management Consolidated Audit Program audit conducted from September 25 through 27, 2000 were also assessed.

There was one finding (missing red tape on a "critical" pipet) and one observation (conflicting data in the electronic bioassay sample status report) noted during the audit. Both were corrected satisfactorily.

3.3.3 Testing of Backup Lab for Rapid Plutonium and Strontium Analyses

Capabilities for performing rapid urinalyses for plutonium and ⁹⁰Sr by PNNL's Radiochemistry Process Group (RPG) were tested twice in 2000. These capabilities are intended to serve as backup for the contract laboratory. RPG staff satisfactorily completed the analyses of the blind performance samples.

3.3.4 Hanford Contractors' 10 CFR 835 Assessment

Contractors are required to assess all functional elements of their radiological protection programs at least once every 3 years. Internal dosimetry and bioassay are considered a single functional element, and the contractors jointly conducted an assessment of HIDP in June, although the assessment letter was not officially issued until August. There were two findings and three observations concerning the HIDP that can be summarized as follows:

- A discrepancy was found between procedure 300-05 and actual practice concerning use of the Bioassay Request Sheet.
- A corrective action plan is needed for completion of the *Methods and Models of the Hanford Internal Dosimetry Program*.^(b)

(a) Nanopure is a registered trademark of Barnstead/Thermodyne.

(b) Pacific Northwest National Laboratory. Current version. *Methods and Models of the Hanford Internal Dosimetry Program*. PNNL-MA-860, Richland, Washington. (Internal manual.) Available URL: <http://www.pnl.gov/eshs/pub/pnnl860.html>

- A need was identified for improved tracking of the timeliness of dose assessments.
- A need was identified to ensure HIDP is aware of and in compliance with contractor radiological control program requirements.
- Three procedures had effective dates preceding signoff dates.

Corrective actions for all of the findings and observations were completed in CY 2000.

3.3.5 Program Self-Assessments

A self-assessment of the program is conducted annually by the program's quality engineer. This year's assessment was conducted in April and found minor discrepancies between actual practice and two procedures, and some procedure training records that had not been completed. Corrective actions were completed by August.

3.3.6 Quality Problem Reports

Four quality problem reports related to bioassay were filed in 2000. These were presented as a group to PNNL's PAAA Working Group in November and were determined to be reportable as a management concern in January 2001. The problems were not entirely within the HIDP, but were isolated cases of breakdown of the complex of systems that together constitute the methods for scheduling, obtaining, and tracking status of bioassay and the prompt reporting of results of concern. Each problem was critiqued when discovered and corrective actions were developed separately. Corrective actions included the following:

- improving the review of the Excreta Bioassay Positive Exam Results Report
- modifying the time period encompassed by the Schedule Due Report (for scheduling in vivo measurements) to scan backward in time to locate workers who had failed to show up for their measurements and failed to get rescheduled
- ensuring that the Grace Period Deficiency Report will identify insufficient volume samples and failed analyses (excreta samples)
- modifying the Daily Sample Excreta Report to include data on insufficient volume samples submitted to the results portion of the REX database (as opposed to being submitted to the excreta status portion of REX)
- modifying the Access Control Entry System (used by FH, CHG, and PNNL for radiological area entry qualifications control) to accept data on insufficient volume and failed analysis samples.

Most of these corrective actions represent improvements to the backup systems for finding data in the database that should have been reported promptly to HIDP. The PAAA Working Group requested two additional corrective actions that were being performed in 2001; one involved corrective actions by the contract excreta bioassay laboratory and the other involved an extensive functional requirements analysis of the whole bioassay system.

3.4 Supporting Technical Studies

Four supporting studies were conducted during 2000, as described in the following sections.

3.4.1 Tritium Absorption Through Skin

A method for calculating dose from uptake through intact skin contact with tritium-contaminated water was developed in response to a contractor request. Based on a water-absorption rate through intact skin of $0.065 \text{ mg/cm}^2\text{-min}$ (Pinson and Langham 1980), the method was documented in a memo to the requesting contractor. It was estimated that 10 minutes of contact with both hands and arms (20% total body skin area) to water contaminated at $641 \text{ } \mu\text{Ci/ml}$ would result in a 100-mrem CEDE. The method will be incorporated into the first revision of the tritium chapter of PNNL-MA-860.

3.4.2 Investigation of a New Internal Dosimetry Code

A computer code, developed by the British National Radiological Protection Board and being marketed in North America by ACJ & Associates, is being considered as a possible supplement or eventual replacement for the CINDY code currently used by Hanford for internal dose calculations. CINDY is now over 10 years old and two significant shortcomings are being experienced with the code: 1) it is limited to the ICRP 30 form of biokinetic models and is not capable of using the new ICRP 66 (1994) lung model or the recent ICRP recycling biokinetic models, and 2) the code is proving to be very difficult to successfully run on current personal computer (PC) operating systems (e.g., Windows 2000 and Windows NT). The Integrated Modules for Bioassay Analysis (IMBA) Code implements the ICRP 66 lung model, recycling biokinetic models, and ICRP 60 weighting factors to give results for intake, retention, and effective dose calculations. Adaptation of these modules to meet DOE requirements of 10 CFR 835 (notably the DOE tissue-weighting factors) would be required; however, the utility of the code and the ability to use the new models (or the former ICRP 30 [1979] models) makes it an attractive possibility and a cost-effective alternative to developing a new code from scratch. In addition, IMBA is designed to run on advanced operating systems and can be easily interfaced with various other applications (e.g., Excel spreadsheets).

Discussions with the vendor, other DOE sites, and DOE-HQ indicated that adaptation of the code to provide a DOE complex-wide version was feasible, and a DOE-HQ (Environmental Health) managed effort to fund the adaptation and development was initiated. HIDP committed \$20K of FY 2001 funding towards this effort. Several other DOE sites have indicated they will provide similar support.

3.4.3 Review of Historical Records on REX

A number of minor modifications to REX internal dosimetry INTERTRAC records were made in preparation for the rehosting of REX. The modifications addressed inconsistencies resulting from changes in reporting criteria and a few data errors that had resulted over the 12 years of INTERTRAC existence. With the expanded use of database queries and provision of database subsets to various researchers, the inconsistency in reporting data was considered likely to lead to errors and inefficiencies in the interpretation and use of data. All assigned internal doses in INTERTRAC were reviewed (1,784 dose entries for 892 evaluations); representing all Hanford workers with internal doses assigned under the ICRP 26 (1977) dosimetry systems as of June 1, 2000. A total of 222 inconsistencies had resulted from the reporting criteria having changed in 1993 from annual dose equivalents to 50-year committed dose equivalents. An additional 12 inconsistencies were identified as errors in the peer review of the evaluation prior to data entry or to previously undetected data entry errors. Memos documenting the modifications were added to each affected worker's file. These modifications brought the INTERTRAC database into internal consistency; with all reported doses being 50-year committed doses.

3.4.4 Bioassay for Hanford Firefighters

A program was established to offer, obtain, and analyze urine samples from firefighters associated with the Hanford range fire of June 29 to July 2. The HIDP initially offered whole body exams to firefighters after the fire prior to leaving the community; however, no firefighters accepted the offer. Later, concerns developed among the firefighters as a result of media reports of elevated environmental air samples and urine sampling was offered to those concerned. Urinalysis requests were received from 53 Hanford employee firefighters and 144 non-Hanford employees and all requesting firefighters were provided sample kits. Of the kits provided, 46 Hanford employees and 71 non-Hanford employees returned samples for analysis. All samples were analyzed for radiostrontium, and 5 samples were also analyzed for plutonium. None of the samples showed any indications of intake.

3.4.5 Review of Draft Basic Ordering Agreement

HIDP staff reviewed a draft basic ordering agreement (BOA) for a DOE complex-wide bioassay procurement and provided comments to the Sample Management Group at the Rocky Flats Environmental Restoration Site, which originated the BOA. The draft resulted from a recommendation by the DOE Inspector General's office 1999 multi-site audit that a DOE-wide contract was feasible and would save money. The HIDP commented that the draft BOA did not meet the analytical sensitivity, turnaround times, quality, or reporting provisions of the current Hanford bioassay contract.

3.5 Project-Related Professional Activities

HIDP staff activities, presentations, and professional memberships during 1999 are listed in this section.

3.5.1 Activities

Donald E. Bihl was Chair of Health Physics Society Standards Working Group N13.39, *Internal Dosimetry Programs*. This working group completed its task when N13.39 was approved by the HPS Standards Committee and the final copy was submitted to the HPS Secretariat for publication.

Eugene H. Carbaugh was involved in professional dosimetry activities, outside of the Hanford Site, as a member of the DOELAP Radiobioassay Oversight Board, and he attended the Board's meeting May 1 to 3 in Idaho Falls, Idaho. He also attended a meeting of the DOE Working Group on Stable Tritium Compounds, from January 18 to 19, in Albuquerque, New Mexico, at which a set of specific issues were identified to be addressed by DOE in establishing policy on radiation protection for metal tritide particulates and organically bound tritium.

Jay A. MacLellan was Technical Program Co-chairman for the 47th Bioassay, Analytical, and Environmental Radiochemistry Conference held in Seattle, November 12-17, 2010.

3.5.2 Presentations

MacLellan, J. A. 2000. "Hanford's Decision Level for Alpha Spectrometry Bioassay Analyses Based on Sample Specific Total Propagated Uncertainty." PNNL-SA-33598, presented at the 46th Bioassay, Analytical, and Environmental Radiochemistry Conference, November 12-17, 2000, Seattle, Washington.

Strom, D. J., D. E. Bihl, E. H. Carbaugh, J. A. MacLellan, and C. L. Antonio. 2000. "Hanford Approach to Dealing with Suspected Intakes of Plutonium." PNNL-SA-34012, presented at the Los Alamos National Laboratory Plutonium Bioassay and Internal Dosimetry Workshop, December 4, 2000, Los Alamos, New Mexico.

3.5.3 Publications

Pacific Northwest National Laboratory. Current version. *Methods and Models of the Hanford Internal Dosimetry Program*. PNNL-MA-860, Richland, Washington. (Internal manual.) Available URL: <http://www.pnl.gov/eshs/pub/pnnl860.html>

3.5.4 Professional Memberships and Other Activities

Carbaugh, E. H., Member of the HPS Standards Committee N13.25, *Internal Dosimetry Standard for Plutonium*.

Carbaugh, E. H., Member Bioassay/ Internal Dosimetry DOELAP Oversight Board.

Carbaugh, E. H., Member DOE Working Group on Stable Tritium Compounds.

MacLellan, J. A., Chair of the American Academy of Health Physics Appeals Committee.

MacLellan, J. A., President-Elect of the Columbia Chapter of the Health Physics Society.

4.0 In Vivo Monitoring Program for Hanford

The In Vivo Monitoring Program for Hanford (IVMP; formerly the Hanford Whole Body Counting Program) has been an integral part of the comprehensive radiological protection program for Hanford workers since 1959. The IVMP staff provides routine and emergency in vivo counting services. The majority of the measurements are performed in the 747-A Building at the corner of Knight Street and Goethals Avenue in Richland. Additional radiation detection equipment is maintained and operated at the Emergency Decontamination Facility located next to the Kadlec Medical Center. Mobile in vivo equipment is also maintained in a trailer located near the 747-A Building. Collectively, the facilities are called the In Vivo Radioassay and Research Facility (IVRRF).

Four shielded counting systems in the 747-A Building were used to perform the routine measurements during 2000. The standup counter employs five large sodium-iodide detectors for measuring fission and activation products in the body with energies >200 keV. It is used primarily as a screening counter to determine whether activity is present above the decision level. The Palmer Room contains a system with seven coaxial high-purity germanium (HPGe) detectors. It is also used to detect and quantify radionuclides that emit high-energy photons. Because of the excellent resolution, it is used to obtain the final results when activity is detected. The Iron Room and Stainless Steel Room each contain planar HPGe detector arrays optimized for the detection of uranium, transuranic radionuclides, and other nuclides that emit low-energy photons. Additional sodium-iodide and HPGe detectors are located in the Lead Room and are infrequently used for organ and whole body counting.

When activity is detected and confirmed, the results are provided to the HIDP to be used in determining the dose to workers from the internally deposited radionuclides. Records of the measurement results, counting system calibrations, and measurement QC records are ultimately transmitted to the Hanford Radiological Records Program. Information copies of the records are maintained at the IVRRF.

The IVMP is accredited through the DOELAP for bioassay and is operated in compliance with 10 CFR 835, *Occupational Radiation Protection*. The program documentation includes the *In Vivo Monitoring Project Manual*, PNL-MA-574,^(a) the *Quality Assurance Plan for the operation of the In Vivo Monitoring Program for Hanford*, LSC-021, and the *In Vivo Counting Program Procedures Manual*, PNL-MA-554.^(b)

4.1 Routine Operations

A total of 6,983 in vivo measurement results were sent to the REX database for DOE and the Hanford contractors during 2000. This included 5,650 whole body measurements, 1,319 chest measurements, and

(a) Pacific Northwest National Laboratory. Current version. *In Vivo Monitoring Project Manual*. PNL-MA-574, Richland, Washington. (Internal manual.)

(b) Pacific Northwest National Laboratory. Current version. *In Vivo Counting Program Procedures Manual*. PNL-MA-554, Richland, Washington. (Internal manual.)

14 miscellaneous measurements. The miscellaneous measurements included wound, skeletal, and thyroid measurements. The total number of counts represents a 14% decrease compared with CY 1999. The reduction is due mainly to the ongoing needs testing being done to remove workers from bioassay schedules if workers did not enter an area requiring bioassay and, in particular, an in vivo bioassay. There were 771 fewer whole body counts performed than in 1999 and 338 fewer chest counts performed than in 1999. The statistical breakdown by contractor is shown in Table 4.1. A summary of the number of in vivo counts made from 1991 through 2000 is presented in Table 4.2 and depicted graphically in Figure 4.1.

Table 4.1. In Vivo Measurements Performed During 2000 and Entered in the REX Database

Count Type and Reason	CHG	FH	PNNL	BHI	Other (DOE and US)
Whole Body Counts					
Routine Schedule	1,057	2,738	564	868	282
Special Request	18	27	1	2	0
Contractor Request	41	20	20	12	0
Total	1,116	2,785	585	882	282
Chest Counts					
Routine Schedule	127	750	244	129	43
Special Request	1	13	5	1	1
Contractor Request	1	1	2	1	0
Total	129	764	251	131	44
Other					
Routine Schedule	0	1	1	0	0
Special Request	4	1	0	3	1
Contractor Request	0	0	2	1	0
Total	4	2	3	4	1
Grand Total	1,253	3,553	842	1,021	328

Table 4.2. In Vivo Count Summary from 1991 Through 2000

Year	1991	1992	1993	1994	1995	1996	1997	1998	1999	2000
WBC ^(a)	9,965	12,197	11,401	11,031	9,020	7,407	6,506	6,478	6,421	5,650
Lung	2,549	3,164	2,838	2,752	1,915	1,632	1,433	1,734	1,657	1,319
Special	66	56	38	82	27	26	4	21	7	14
Total	12,580	15,417	14,277	13,865	10,962	9,065	7,943	8,233	8,085	6,983
(a) Whole body count										

The IVMP operated within budget in 2000. Work was scheduled and prioritized at regularly scheduled planning meetings. Monthly safety meetings were conducted to address program-specific topics. Quarterly safety self-assessments were conducted. No off-normal events were recorded. Each quarter, formal presentations were made to RL and the contractors to summarize the status of the program. The measurement QC data were reviewed and analyzed for quarterly trends.

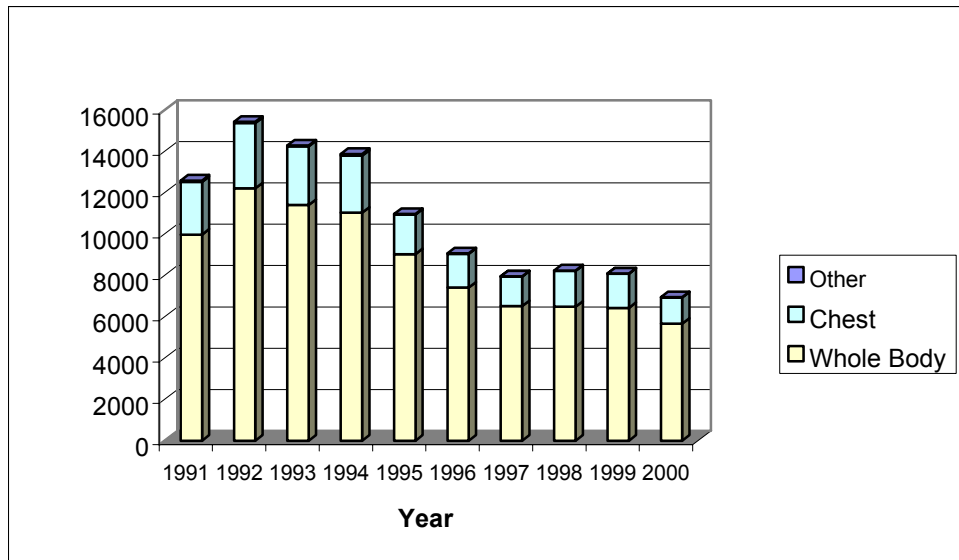


Figure 4.1. Summary of the Number and Types of In Vivo Measurements Performed from 1991 Through 2000

The daily QC measurement results indicated that the calibration factors based on the measurements of the calibration phantoms were applicable to all of the official measurement results recorded in CY 2000. In the rare cases where the daily QC results were out of tolerance, worker data were reviewed for validity and when necessary workers were scheduled for recounts.

There were no millennium transition-related problems associated with the startup of the Abacos software on January 3, 2000.

4.1.1 Program Documentation

Three internal PNNL program manuals were updated during the year. Sections 2.0, 3.0, 4.0, 5.0, 7.0, and 8.0 of PNL-MA-574, *In Vivo Monitoring Project Manual*, were updated to reflect changes made when the Abacos software was put into routine use.

Revision 5 of the *QA Plan*, LSC-021, was issued in September. The changes, which resulted from the annual review of the plan, updated the information on the organizational structure and clarified existing requirements.

The operating procedures in PNL-MA-574 were revised on an as-needed basis to ensure that the procedures accurately reflect the methods used to perform the work.

4.1.2 Department of Energy Laboratory Accreditation Program

The initial DOELAP accreditation expired in February 2001. In 2000, routine operations were conducted using the Abacos Plus software loaded on a Compaq Model 255 Workstation running the VMS operating system. Technical equivalence was granted by DOELAP for routine operations with Abacos Plus in all six categories. The technical equivalence demonstrated that operations with Abacos Plus had at least the same degree of quality compared with the previous NEXEC system, which was used to obtain the initial DOELAP accreditation in 1998. The IVMP staff completed performance testing in six categories and met the bias and precision criteria in all six. The performance test results are shown in Table 4.3. The onsite assessment was conducted on January 15 and 16, 2001. There were no deficiencies, only one concern, and seven observations noted during the assessment. Deficiencies will prevent accreditation of the program until they are corrected; a concern is a programmatic issue that doesn't currently compromise the program but requires a corrective action plan; and observations are suggestions to improve the program or noteworthy practices. Observations do not require a corrective action plan. One of the seven observations noted was a noteworthy practice. The corrective action for the one concern simply involved adding a list of equipment to two calibration records and was completed. The formal response was transmitted to DOELAP. Although not required, responses to the six observations were prepared.

Table 4.3. Results from CY 2000 DOELAP Performance Testing^(a)

Test Category	Result ^(b) (nCi)	nCi in Phantom	Relative Bias	Relative Precision
²⁴¹ Am in lungs IR	40.8	41.1	-0.007	0.027
²⁴¹ Am in lungs SS	40.2	41.1	-0.022	0.02
²³⁹ Pu in lungs IR	768	846	-0.092	0.026
²³⁹ Pu in lungs SS	770	846	-0.090	0.019
²³⁴ Th in lungs IR	24	25.4	-0.055	0.028
²³⁴ Th in lungs SS	23.6	25.4	-0.071	0.053
²³⁵ U in lungs IR	3.92	4.42	-0.113	0.025
²³⁵ U in lungs SS	3.90	4.42	-0.118	0.016
¹³⁴ Cs (WB) SU	1040	786	0.323	0.04
¹³⁴ Cs (WB) CC	798	786	0.015	0.01
¹³⁷ Cs (WB) SU	728	793	-0.082	0.04
¹³⁷ Cs (WB) CC	842	793	0.062	0.01
⁶⁰ Co in lungs CC	813	782	0.039	0.01
⁵⁴ Mn in lungs CC	980	937	0.046	0.008
(a) IR = Iron Room SS = Stainless Steel Room WB = whole body SU = standup counter CC = coaxial HPGe counter (b) Average of 5 measurements				

4.1.3 Equipment Maintenance and Repair

Three HPGe detectors required repair during the year. Other electronic components that also were repaired included:

- 11 main amplifiers
- 3 nuclear instrument module (NIM) bins
- 1 high-voltage power supply
- 1 preamplifier power supply

This resulted in an estimated \$15,000 cost savings compared with shipping the detectors and electronic components offsite for repair. One NIM bin that was still under warranty was returned to the factory for repair.

The portable counting system described in last year's annual report consists of a 28-cm² by 20-mm-thick planar HPGe detector, a laptop computer, and a single electronics module. The system was calibrated for low- and high-energy wound counting this year. The low-energy configuration has a conversion gain of 0.25 keV/channel with 2,048 channels for counting of nuclides that emit photons with energies up to 200 keV. The high-energy configuration has a conversion gain of 1.5 keV/channel using 2,048 channels to detect and quantify nuclides that emit photons with energies up to 3 MeV. The system has proven to be very stable. The MDAs for americium and plutonium in a shallow puncture wound are 10 pCi and 200 pCi, respectively. The operating procedure was written and staff were trained on the operation of the counting system.

A new Access database was developed to document instrument and detector repair histories. The Access database replaces the "Yourway" card file software that had no user documentation. The database allows the maintenance histories to be accessed by equipment type and property number.

The battery capacity of the uninterruptible power supply system was checked and found to be adequate to provide sufficient (40 to 50 minutes) backup power to allow shutdown of the critical instrumentation during business hours.

In September, the amount of time required to transfer and save the spectral configurations to the Alphastation disk began to increase for the standup and coaxial counters. At times, 2 to 3 minutes are required to completely save the configurations to disk. The chest-counting systems take much less time to complete the same "transfer and save" process. Two VMS utilities, Autogen and Monitor, were run to optimize system parameters. The optimization had little impact on the times required to save the spectral configurations. The system memory was increased from 96 Mb to 256 Mb again with no observable increase in the processing speed. It appears that reducing the number of files stored on the user disk will be required to improve the processing speed. A direct connection to LaserREX will be established in CY 2001 to facilitate removing the files.

The seven rectangular NaI detectors from the mobile counter were installed in the Lead Room. A lie-down counter was fabricated using the detectors to serve as a backup to the standup counter. The system was tested and found to be ready for acquiring data. It will take a week to ready the system for routine operation if needed.

4.1.4 Facility-Related Activities

The 747 Building complex was sold to Mr. James Go in June. The IVMP currently has a 5-year lease agreement to occupy the 747-A Building with options for two additional 5-year extensions. The owner promptly addressed all facility issues that occurred since June.

4.1.5 Historical In Vivo Measurement Records

With assistance from PNNL Information Systems, the Oracle database was restored to the pre-crash configuration that contained records through October 21, 1999. The database contained the records for all the in vivo measurements performed from March 1995 through October 21, 1999. The records were saved to compact disks (CDs) in ASCII format and Oracle (Version 8.1.6) format for future access. The Oracle format will allow access in the near future (3 to 5 years) and the ASCII format will allow retrieval of the data for the foreseeable future. Explanations of the data format were generated and included on the CD.

4.2 Program Changes and Improvements

The first full year of operation using the Abacos Plus software was completed in CY 2000. Overall, the system operated reliably. Several programs were written to provide customized tools for error checking, data handling, and analysis of data. Code was written to 1) perform mean blank value analyses, 2) evaluate the false positive rate, 3) add multiple spectra, 4) eliminate the generation of duplicate tagwords, 5) monitor the number of files transferred to REX, and 6) check the tagword sequence to help identify whether there are any missing records. In addition, a new plotting routine with much better resolution than the standard Abacos Plus plotting package was added as an option.

Shielded cables were fabricated and installed for the coaxial HPGe motion control system to reduce the level of electromagnetic interference generated by the operation of the motion controller. The interference contributed to the background count rate in the low-energy region and also degraded the system resolution.

On December 11, the three ADIT photomultiplier tubes (PMTs) on the 11.5-inch sodium iodide detector used on the standup counter were replaced. This detector was experiencing changes in gain that were inversely proportional to the temperature. The new PMT manufactured by Hamamatsu, Inc. reduced the ^{40}K background level, and more importantly, stabilized the troublesome gain drift (inversely proportional to temperature) associated with the other PMT. The QC parameters for ^{40}K were adjusted to account for the decrease in the potassium activity.

Four digital signal-processing (DSP) units were installed in the Stainless Steel Room. One DSP replaces an amplifier and an analog-to-digital converter. The four DSP together eliminate the need for a multiplexer. This system will allow individual detector start/stop control and may improve system performance. A digital signal is transmitted from the Counting Room to the multichannel analyzer (MCA) located 30 feet away in the instrument rack; this eliminates amplification of analog noise signals from the cable. The DSP arrangement was configured on the Abacos Plus software for data acquisition and tested. Preliminary results indicated that the system was operating properly. More extensive testing is scheduled for CY 2001.

The chest-counting calibration was extended to 5.3 cm from 4.1 cm by combining two overlays. This was done to account for the customers who have a predicted chest-wall thickness greater than 4.11 cm based on their weight-to-height ratio. If activity were detected above the L_c then the chest-wall thickness (CWT) would still be estimated using ultrasonic measurements.

The manually operated assemblies for adjusting the attitude of the four detector arrays in the two chest-counting systems were replaced due to normal wear and tear from routine use. In addition, the micro switches for the Stainless Steel Room doorstop were replaced.

A model was developed of a chest counting system and a source jig used for the daily QA checks using the Monte Carlo N-Particle (MCNP) transport code. The empirical and MCNP spectra are very similar with some variance in the MCNP data at certain energy ranges compared to the empirical data. This may be simply a matter of running more tallies with MCNP. The next step is to model a phantom with a radioactive material distribution and use MCNP to transport photons from a source organ to the detector.

4.3 Program Assessments

Representatives from the Hanford contractors' dosimetry organizations conducted the triennial assessment of the in vivo and internal dosimetry programs June 12 through 14 as part of the ongoing sitewide self-assessment process. There were two findings and six observations related to the in vivo program. Action plans for the findings and observations were completed.

A procedure compliance surveillance was conducted as part of the 2000 management assessment. Corrective actions for the findings were completed.

Representatives from U.S. Ecology (USE) conducted a one-day audit of the program. No findings resulted from the audit. The IVMP remains on the USE-approved vendor listing for in vivo services.

4.4 Supporting Technical Studies

Six supporting technical studies were undertaken during 2000, as described in the following sections.

4.4.1 Thyroid Radioiodine Intercomparison Program

The results from participation in the Thyroid Radioiodine Intercomparison Program (TRIP) are shown in Table 4.4. The bias for the ^{125}I results was 5% or less. There were three quarters where the ^{131}I measurement bias was 5% or less and one quarter where the ^{131}I bias was -14%. All results were well within the DOELAP bias criteria.

Table 4.4. Results from the Thyroid Radioiodine Intercomparison Program

^{125}I Result (dpm)	^{125}I True Activity (dpm)	^{125}I Bias	^{131}I Result (dpm)	^{131}I True Activity (dpm)	^{131}I Bias
4 th Quarter 1999					
8.06E+05 ± 9.8E+04	8.32E+05 ± 2.5E+04	-0.03	1.05E+06 ± 2.5E+04	1.07E+06 ± 3.22E+04	-0.02
1 st Quarter 2000					
7.23E+05 ± 1.2E+05	7.51E+05 ± 2.25E+04	-0.04	1.93E+05 ± 3.03E+04	2.24E+05 ± 6.73E+03	-0.14
2 nd Quarter 2000					
2.78E+05 ± 2.92E+04	2.92E+05 ± 8.76E+03	-0.05	2.59E+06 ± 3.89E+04	2.72E+06 ± 8.16E+04	-0.05
3 rd Quarter 2000					
2.49E+05 ± 2.46E+04	2.52E+05 ± 7.56E+03	-0.01	2.00E+05 ± 1.20E+04	2.01E+05 ± 6.03E+03	0.00

4.4.2 Thoron In-Breath Monitor Study

Preliminary discussions were held with Pylon, Inc., to address the transfer of the thoron-in-breath technology. Battelle is mailing a brochure describing the thoron in-breath monitor (TIBM) to potential customers. Pylon is beginning an analysis of the potential market for the TIBM.

4.4.3 Measurement Quality Control

As part of the ongoing measurement QC program, measurements are performed to estimate the activity content of phantoms as they become available. These phantoms may come from various sources and their activity is not known to the IVMP staff prior to making the measurements. The result from the measurement with a chest-counting system of a natural uranium lung phantom was 186 nCi versus a stated activity of 185.8 nCi. The result is within 0.1% of the stated activity in the phantom.

Measurements were also made of calibration phantoms during the year. Figure 4.2 illustrates the bias from measurements of two sets of ^{241}Am lung phantoms. All results were within 9% of the stated activity in the phantom.

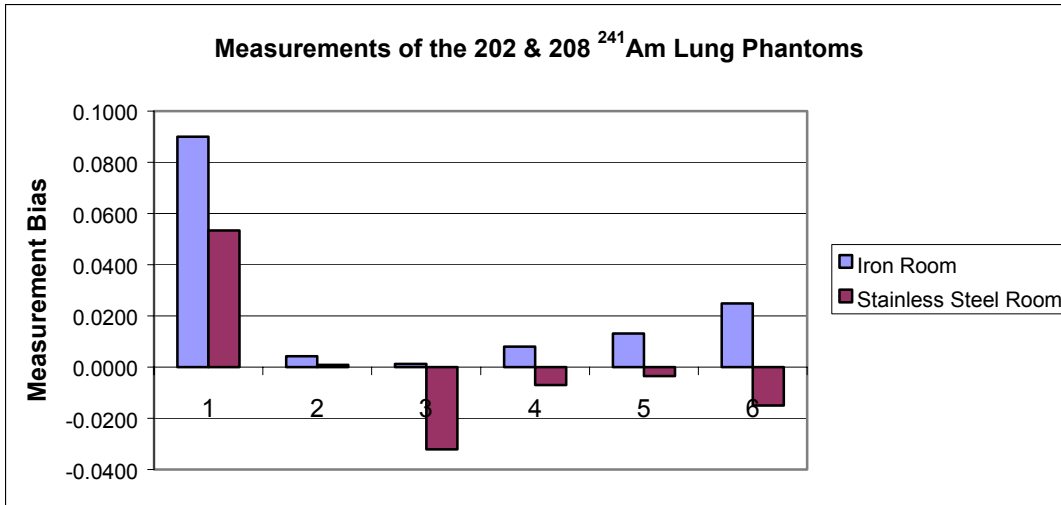


Figure 4.2. Lung Phantom Quality Control Results

4.4.4 Measurements of Thallium Following Medical Administration

Measurements were made over a 57-day period on an individual who received 4.1 mCi of ^{201}Tl for a diagnostic medical study. Measurements were performed periodically to evaluate the interference to the routine lung and whole body counting systems. The initial measurements were made 6 days after the injection; significant dead time was exhibited on both the coaxial HPGe system and the lung-counting system in the Stainless Steel Room. Two of the lung-counting detectors in the Stainless Steel Room exhibited degraded resolution at the high count rates. In addition, the L_c values for the routine lung counting nuclides ^{234}Th , ^{241}Am , and ^{235}U were 1000x, 100x, and 40x typical values, clearly levels where a valid measurement was not possible. Figure 4.3 illustrates the net count rate measured with the four planar HPGe detectors in the Stainless Steel Room as a function of time after injection. The deviation

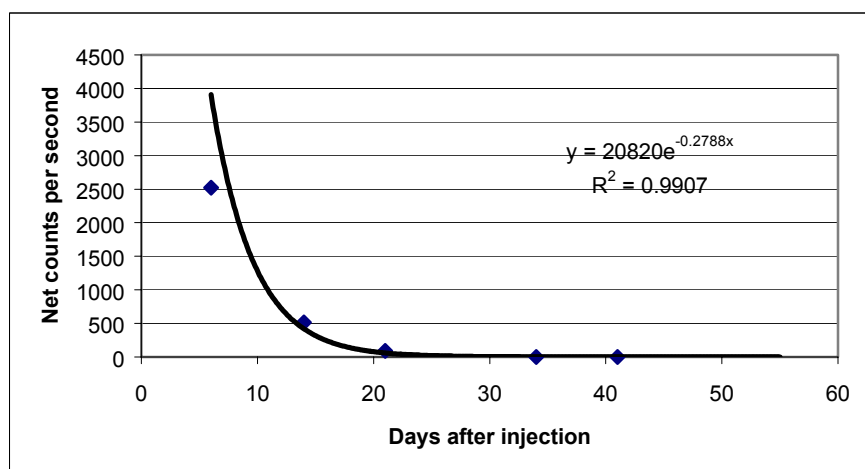


Figure 4.3. ^{201}Tl Net Peak Count Rate at 167 keV

from the fitted curve caused by the high-count rate at 6 days after injection is clearly seen. At 57 days after injection, the L_c values were two to three times higher than the expected values due to interference from the ^{202}Tl activity. The ^{202}Tl is an impurity, generated by the cyclotron production of ^{201}Tl , with a half-life of 12 days compared to the 73-hour half-life of ^{201}Tl .

At 6 days after injection, the standup counter spectrum contained a huge continuum from the thallium activities that actually contributed to the ^{137}Cs and ^{154}Eu results exceeding the L_c . The decision levels for cesium, cobalt, and europium were also a factor of two higher than usual. At 21 days after injection the dead times on the coaxial HPGe system and the standup counter were minimal. Figure 4.4 illustrates the count rate measured with the coaxial HPGe system at different times after injection and again the deviation from the fitted curve caused by the high count rates is apparent. The study results suggest that a worker should wait 3 months after a thallium injection of 4 mCi or more before getting a chest count and 3 weeks before getting a whole body count. Effective half-lives of 3 days and 9 days were calculated for ^{201}Tl and ^{202}Tl , respectively, in this case.

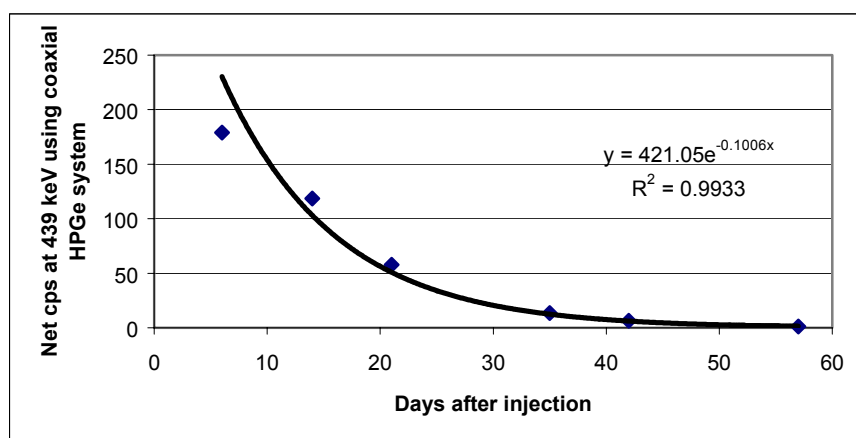


Figure 4.4. ^{202}Tl Count Rate Versus Time After Injection

4.4.5 $^{241}\text{Am}/^{152}\text{Eu}$ Lung Phantom and Coincidence Summing

An attempt was made to use a single lung phantom containing ^{241}Am and ^{152}Eu to calibrate the chest-counting systems in the Iron Room and the Stainless Steel Room. Unfortunately, when the Am/Eu calibration was validated with the ^{235}U lung phantom it was discovered that the ^{235}U activity was over-estimated by 25%. It was determined that the coincidence-summing phenomenon was the cause. Coincidence summing results when two photons deposit their energies in the sensitive volume of the detector within the counting system's resolving time. Consequently, a peak is formed with an energy equal to the sum of the two incident photons and counts are lost at the energies of the two incident photons. This summing produced a smaller value for the calibration factor in the energy range of 100 keV to 200 keV. A comparison of the Am/Eu calibration curve with a curve generated from measurements of single nuclide lung phantoms (americium and uranium) is shown in Figure 4.5. The figure illustrates graphically the 25% difference in efficiency at 185 keV. A collaborative effort with two

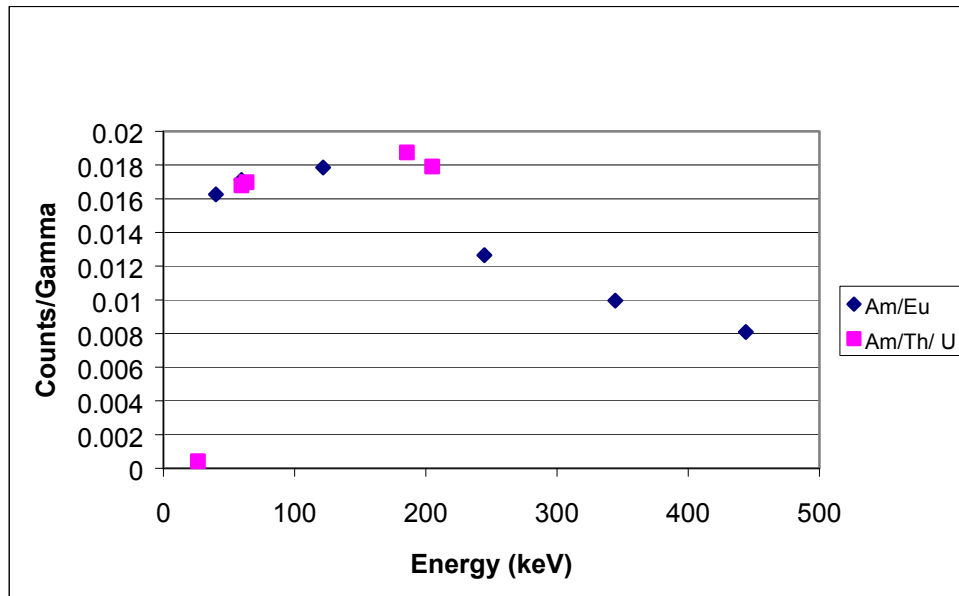


Figure 4.5. Efficiency Calibration Comparison

other laboratories experiencing the same phenomenon was started to further research this phenomenon. Calibration of the chest-counting systems continues to be performed using a ^{241}Am lung phantom, a ^{nat}U lung phantom, and a ^{235}U lung phantom.

4.4.6 Check Source Anomaly

Platinum X-rays were observed in the ^{152}Eu source (#452) used for the daily performance checks in the Iron Room. The X-rays are produced from photoelectric interactions with the platinum in the platinum-clad nickel backing for the source. Curiously, the measurement spectra of the other supposedly identical ^{152}Eu source (#453) used in the Stainless Steel Room do not contain the 65-keV and 67-keV X-rays. The vendor (Isotope Products Laboratory) indicated the problem probably involved the poor quality of the backing material and may even be due to the lack of platinum added to the nickel. The platinum is added to increase the corrosion resistance of the nickel backing material. Contamination surveys and the daily counting results indicate that the integrity of both sources has not been compromised. At this time the peaks do not represent an interference problem with the daily efficiency checks performed with the source.

4.5 Program-Related Professional Activities

Staff activities, presentations, and professional memberships during 1999 are listed in this section.

4.5.1 Activities

Tim P. Lynch was the lead assessor for the onsite DOELAP assessment at the Idaho National Engineering and Environmental Laboratory.

The IVMP staff hosted Alexander Efimov from the Mayak facility in Russia. Mr. Efimov came to learn more about the IVMP operations with the Abacos system. He is using the PC version of Abacos at his facility. The Mayak facility uses HPGe detectors and a shielded room obtained from the DOE Rocky Flats site for counting.

In response to the fire that swept the site in late June, plans and preparations were made to count a large number of firemen in a short time. However, the need never materialized because few firefighters opted to receive the counts. The IVMP staff worked many overtime hours in order to extend the in vivo counting service to the firemen.

4.5.2 Presentations

Tim P. Lynch presented “Thoron Breath Monitoring” to the DOE Air Monitoring Users Group Meeting on March 23. The presentation included a demonstration of the operation of the TIBM.

Tim P. Lynch presented the paper “Coincidence-Summing with $^{241}\text{Am}/^{152}\text{Eu}$ Lung Phantoms” at the DOE Lung Intercalibration Committee meeting in May at Idaho Falls.

4.5.3 Publications

Lynch, T. P., D. E. Bihl, M. L. Johnson, J. A. MacLellan, and R. K. Piper. 2000. *Hanford Radiological Protection Support Services Annual Report for 1999*. PNNL-13238, Pacific Northwest National Laboratory, Richland, Washington

5.0 Hanford Radiation Records Program

The Hanford Radiation Records Program (HRRP) supports RL and Hanford contractor radiation protection programs by administering and preserving radiological exposure records for all Hanford workers and visitors, past and present, and by providing specified and requested reports using these records. The program is also responsible for maintaining the Hanford Radiation Protection Historical Files; operating the computer systems and library equipment necessary to input, store, verify, and retrieve the records; and producing the required reports and downloads. Although data processing functions are now the responsibility of Dosimetry Services, data entry and validation are reported in this section.

5.1 Overview

The HRRP is organized into four major functional areas: data administration, data processing, report issuance, and the Records Library, as described in the following sections. Data processing and part of report issuance are performed by the HRRP Dosimetry Services Dosimetry Operations.

5.1.1 Database Administration

The database administrators evaluate systems, troubleshoot, resolve system and user problems, train users, oversee system security, serve as liaisons with the computer analysts, and initiate and test modifications of the databases for the REX database and Access Control Entry System (ACES). The ACES data administrator provides monthly reports of entry and dose data to PNNL and FH. Upon request, the data administrator also provides personnel qualification reports to federal and state regulators, and adjusts the Administrative Control Limits (ACLs) for individuals in accordance with established policies. The data administrator monitors data downloads for accuracy, and is the point of contact for access qualification or system problems. The data administrator also initiates, tracks, and participates in the evaluation and review of system change requests.

The ACES was created to implement a system for computerized supplemental dose tracking and radiation area/hazardous waste site access control. It is a computerized access control program that electronically compares worker qualifications with controlled area access requirements. Although HRRP has data administration responsibilities for ACES, FH retains ownership. However, the HRRP manager works closely with the FH ACES manager and Lockheed Martin Services, Inc., (LMSI) personnel in the operation and maintenance of the system. ACES is a client-server system, hosted on an HP 9000 computer (four 180-MHz processors) using the Hewlett Packard Unix operating system and Oracle software to manage the database and provide entry screens and reports. Users access the server via PCs connected to the Hanford Local Area Network (HLAN) using Windows-based software residing on the users' (clients') computers. The database receives data from several other Hanford computer systems (e.g., PeopleSoft, REX, and PeopleCORE).

The REX system is a computerized database that maintains all of the radiological exposure records and supplementary and support data for individuals who have worked at the Hanford Site since 1946.

The REX system contains the individual radiological exposure records on all Hanford DOE, contractor, and subcontractor employees as well as Hanford visitors. The system also contains other information used by site radiation protection organizations such as individual skin contamination reports and bioassay schedules and delivery addresses. These data are readily retrievable via a system of PCs and terminals operated by the HRRP and Hanford contractor dosimetry staffs. The REX system also includes supporting exposure documentation on microfilm and CD that are indexed into computer-assisted retrieval (CAR) systems. The CAR systems allow for rapid retrieval of the documents for any individual person using identifiers (IDs). These IDs include payroll numbers, social security numbers, names, and/or REX IDs, which are unique numbers generated by the computer for each individual to tie all of their records together. The HRRP also uses a CD imaging subsystem for hard-copy documents. The imaging and storage hardware is used by two systems, a personnel exposure document system (LaserREX), and an instrument calibration record system (LaserCAL). Since January 1, 1992, all hard-copy exposure records have been preserved on LaserREX. Hard-copy records generated prior to 1992 are maintained on microfilm. The LaserREX also stores the electronic records created by the REX transaction log subsystem, which logs all changes to the database data fields.

5.1.2 Data Processing

Data processing includes entering data into the REX database and validating all data entry. This function is actually the responsibility of the Dosimetry Processing Center for DOE and FH data, and PNNL Safety and Health Technology and Bechtel Radiological Control for their own data. Data validation is accomplished by reviewing field data entry, establishing audits to be matched to entries of results, resolving unmatched results, and interacting directly with contractor personnel. Data handlers also deal directly with contractor personnel and data suppliers to assist them and solve data problems. The Dosimetry Processing Center also issues, tracks, and processes dosimeters for FH and DOE.

5.1.3 Report Issuance

The report issuance function is shared by HRRP and the Data Processing Center. The Data Processing Center is responsible for generating and issuing routine exposure status reports to the contractors, quarterly person-rem and annual statistical reports to DOE, and annual reports to employees. This function requires close contact with RL, the contractors, and other personnel dosimetry functions. Special reports requested by former employees, as well as those requested by the contractors, RL, the United States Uranium and Transuranium Registries, and Privacy Act and Freedom of Information Act petitions are the responsibility of HRRP.

5.1.4 Records Library

The Records Library maintains individual exposure records and backup documentation that are not reducible to database elements, as well as the HRRP Historical Files. The library staff scan, index, and retrieve hard-copy documents; prepare documents for long-term storage; and track and account for the documents through the imaging and indexing process. The library contains the individual exposure records of all Hanford personnel since Hanford's inception in 1944 (almost five million microforms),

except for those individuals who transferred from Hanford when DuPont left in 1946. These exposure records and the Historical File microforms are retrievable through index systems that are maintained by the library staff.

Although the results from the dosimeter and excreta processing, as well as the in vivo counts, are received by electronic transmission, a large amount of data is entered manually by the field dosimetry organizations and the Data Processing Center staff. The hard copies are then sent to the library for preservation on the imaging systems. Records in the HRRP Historical Files include documents such as policies, procedures, reports, and important communications that define the Hanford radiological dosimetry and radiation protection programs throughout their history. The historical records are microfilmed and indexed into an additional CAR system. These records are retrievable by author, date, or range of dates, document number (if applicable), document title, and up to three keywords.

Starting September 20, 1999, the LaserREX document scanning and retrieval hardware was shared with a new document database for Instrument Services and Technology, LaserCAL. The system was cloned from LaserREX, and is operated by the Records Library staff.

The program is operated under the applicable sections of 10 CFR 830 and 10 CFR 835; ANSI N13.6, *American National Standard Practice for Occupational Radiation Exposure Records Systems* (ANSI 1999); as well as the following DOE directives: DOE Guide 1324.5B, *Implementation Guide for Use with 36 CFR Chapter XII - Subchapter B Records Management* (DOE 1996); DOE Guide 441.1-11, *Occupational Radiation Protection Record-Keeping and Reporting Guide* (DOE 1999c), DOE Order 231.1-1, *Environment, Safety and Health Reporting* (DOE 1997); and DOE Manual 231.1-1, *Environment, Safety and Health Reporting Manual* (DOE 2000). The program also complies with the applicable sections of the Privacy Act (1974) and the Freedom of Information Act (FOIA 1966).

5.2 Routine Operations

Staff routinely administer and process data, issue reports, and maintain the Records Library.

5.2.1 Data Administration

Over 2441 Radiation Work Permits (RWPs) were created/closed in ACES in 2000, and over 252,603 access instances occurred. The REX database administrator completed 56 software change requests in 2000 to REX Version 2, and an additional 11 to Version 3 after implementation in October.

5.2.2 Data Processing

In most categories, the number of documents sent from the Data Processing Center to the HRRP records library decreased from 1999 totals (see Table 5.1). However, the total number of documents scanned increased by 50 percent. The increase was due to operation of LaserCAL for the full year, and the decision to enter the "Report of Hanford Occupational Radiation Dose Status" (report card) in the LaserREX system for each person.

Table 5.1. Data Processing Center Activity for Calendar Year 2000^(a)

Document Type	Number Processed	
	1999	2000
Personal Radiation Exposure History Form (used to document exposure history prior to Hanford and to initiate a record for a new or rehired employee)	3,050	2,471
Employee and Dosimetry Change Forms (used to document personnel data or dosimetry changes)	11,340	7,191
Termination Letters (used to document employee terminations, many changes were done electronically not requiring forms)	1,221	1,320
Temporary Dosimeter Assignment Forms (used for issuing temporary dosimeters to employees due to new hires, changes in dosimetry requirements, multiple dosimetry needs, or employees who forgot their dosimeters)	5,090	5,125
Visitor and Subcontractor Dosimeter Issue Forms (used to issue dosimetry to visitors and subcontractors who have not completed radiological worker training)	2,189	1,689
Investigation of Dosimeter Result Forms and Change Letters (used to estimate exposure for lost, damaged, or otherwise suspect dosimeter results)	743	494
Special Process Forms (used to document data for specially processed dosimeters)	1,672	4,391
(a) These document totals are included in the records library summary below for records scanned and indexed into LaserREX.		

A discrepancy report, developed in 1999, that compares REX data with security data identified a number of name discrepancies. As each error was corrected, a change form was produced and indexed. About 1500 errors were identified and corrected in 2000.

5.2.3 Report Issuance

As shown in Tables 5.2 and 5.3 and Figures 5.1 through 5.4, work was relatively consistent with 1999.

Table 5.2. Number of Responses to Requests for Previous Exposure

	1999				2000			
	1 st Qtr	2 nd Qtr	3 rd Qtr	4 th Qtr	1 st Qtr	2 nd Qtr	3 rd Qtr	4 th Qtr
Miscellaneous	26	7	0	0	36	0	0	25
Privacy Act/FOIA Requests	7	5	1	1	11	20	9	10
From Current Employees	7	1	4	2	3	4	1	4
From Former Employees	2	0	0	0	2	1	4	2
From Companies	47	120	84	43	35	35	65	50

Table 5.3. Number of Visitor Exposure Letters

	1999				2000			
	1 st Qtr	2 nd Qtr	3 rd Qtr	4 th Qtr	1 st Qtr	2 nd Qtr	3 rd Qtr	4 th Qtr
DOE-HQ	12	24	35	40	18	28	18	17
DNFSB ^(a)	7	4	14	13	7	2	9	13
IAEA ^(b)	6	7	7	8	4	5	5	10
Miscellaneous	--	507	667	437	294	383	357	389

(a) DNFSB = Defense Nuclear Facility Safety Board
(b) IAEA = International Atomic Energy Agency

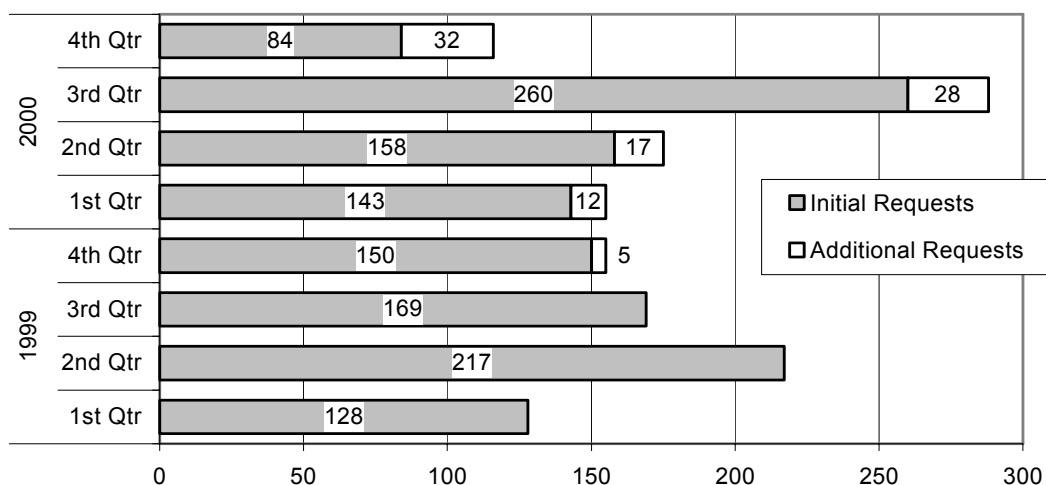


Figure 5.1. Number of Requests for Previous Exposure

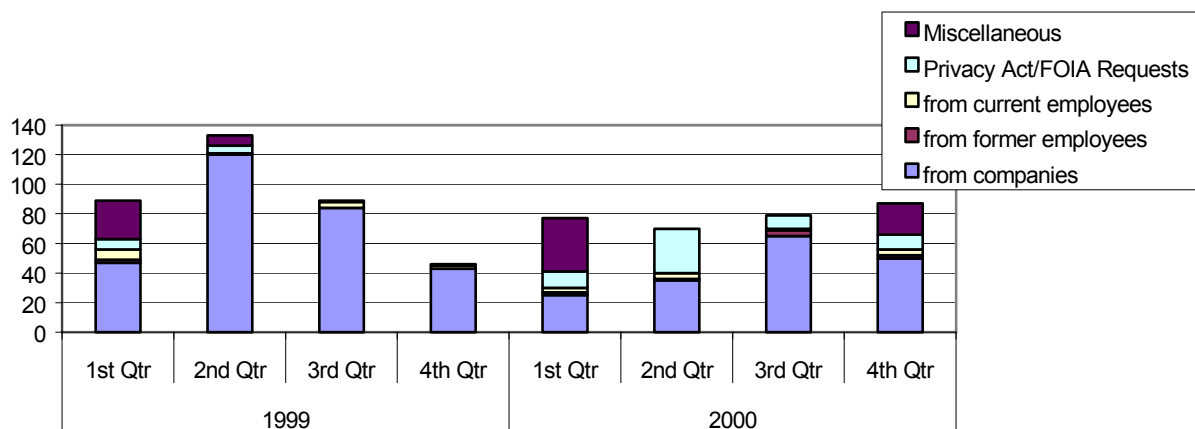


Figure 5.2. Number of Responses to Requests for Previous Exposure

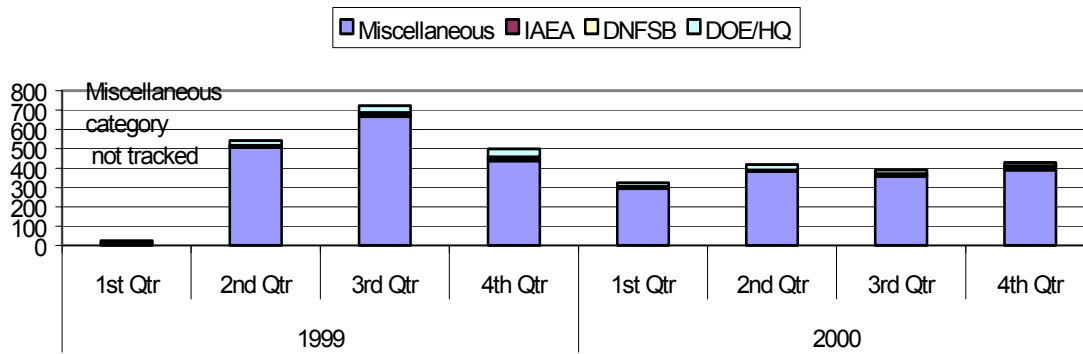


Figure 5.3. Number of Visitor Exposure Letters

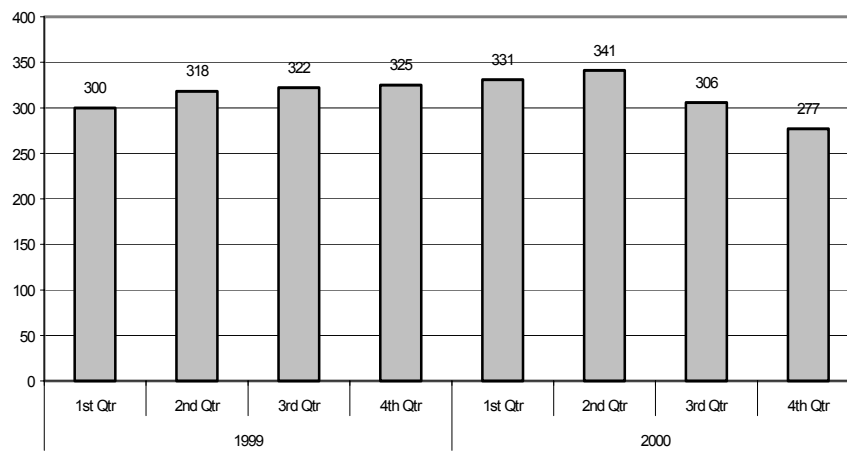


Figure 5.4. Number of Termination Letters

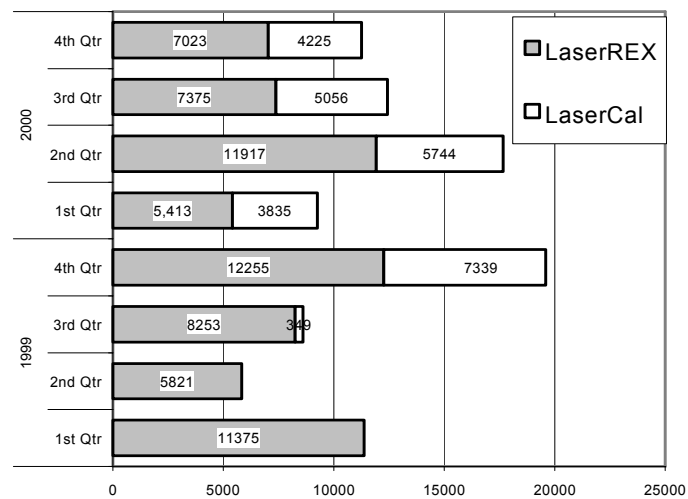


Figure 5.5. Number of Documents Scanned/Indexed

5.2.4 Records Library

The number of documents scanned and indexed into the LaserREX and LaserCAL systems this year was up 11% from 1999, to about 50,000 documents. This was the first full year of operation of the LaserCAL system, which accounted for over one-third of the Records Library workload in 2000. Additionally, all "Report of Hanford Occupational Radiation Dose Status" (report card) documents were entered into the LaserREX system for the first time in 2000, adding about 7,500 documents scanned. These additions more than offset a decrease of 16% in the number of LaserREX documents scanned in 2000.

5.3 Program Changes and Improvements

Database and document scanning capabilities were improved during the year, as described in the following sections.

5.3.1 ACES Database

The original version of ACES was determined to not be Year 2000 (Y2K) compliant. Therefore, an upgrade (Version 6.0) was initiated in 1998 that maintained the established functionality, but in a Windows-based client-server environment that is fully Y2K compliant. The new system was implemented in early 1999. The ACES data administrator was very involved with testing screens and reports in Version 6.0 prior to its release, coordinating user field testing, developing the user manual, and training the users on the new system. ACES did not encounter any significant Y2K problems as it transitioned into the new year.

In May 2000, ACES 6.5 was released with the upgrade to Oracle Developer 6.0, which included Oracle Forms Version 6.0 and Oracle Reports Version 6.0, to be compatible with the new REX Oracle Runtime and Development tools. In the third and fourth quarters of 2000, efforts were concentrated on the development of ACES 7.0, which allows the incorporation of external equipment to the ACES computers, such as the electronic dosimeter readers, brick (pseudo dosimeter) label printers, and bar code readers.

5.3.2 REX Database

Battelle, along with the major REX users, agreed in 1999 that the system needed to be redeveloped/re-hosted into a more cost-effective environment, and a contract was signed with the Science Applications International Corporation (SAIC) to redevelop the system. The user interface was developed using the Oracle Developer 2000 suite of tools. The Oracle-based client server system was released for production use on October 2, 2000. The REX Version 2 database was migrated from a DB2 database, residing on an IBM mainframe computer to an Oracle database (REX Version 3), residing on a UNIX platform on a Sun Microsystems Enterprise server operated by PNNL. The last REX-related system on the IBM mainframe computer was removed in December.

The REX database performed very well all year (both Version 2 and Version 3). Software Change Requests (SCRs) were kept to a minimum to avoid having to coordinate and implement new code in both systems. However, during the re-hosting effort, each of the processes, screens, and reports were reviewed and modified as identified by the REX users. Most of the SCRs issued during the year were for changes and enhancements to make the operations more efficient and data entry less cumbersome. The REX User's Group, initiated late in 1993, was instrumental in proposing and defining many of the enhancements and changes.

The REX database administrator and the LMSI maintenance programmer completed 56 software change requests for REX Version 2 in 2000, before a moratorium was placed on REX changes the end of April, in anticipation of the REX Version 3 migration. SCR work was resumed on REX Version 3 the end of October, and 11 additional SCRs were completed in 2000. Some of the significant changes included the following:

- corrected screens, reports, and programs to reflect the mass personnel transfers from B&W Protec, Inc. to Protection Technology Hanford, and LMSI to CHG.
- revised the format of the visitor and termination letters
- provided automated notifications to ACES when processes did not run as expected.

5.3.3 Document Scanning

The LaserREX system consists a single 350-MHz dual processor Gateway ALR 7200 server using Windows NT, coupled with two computer workstations, each with an optical scanner. There were no major periods of unavailability this year.

LaserCAL uses existing LaserREX hardware with modified software cloned from LaserREX. LaserCAL provides a retrievable document database for the Instrument Services and Technology Project. About one-third of the documents scanned and indexed by Radiation Records are now for the Instrument Services and Technology Project. The Hanford Identification Number was added to the keywords of the LaserREX system in 2000. This was necessary because of the planned elimination of the Payroll ID number by the Hanford Site.

5.4 Program Assessment

There were no assessments or surveillances of Radiation Records performed during 2000.

5.5 Supporting Projects

None

5.6 Program-Related Professional Activities

Jay A. MacLellan served as:

- Chair of the American Academy of Health Physics Appeals Committee.
- President Elect, Columbia Chapter of the Health Physics Society (from June 2000).

6.0 Instrumentation Services and Technology Program

The Instrumentation Services and Technology Project (IS&TP) provides complete and reliable calibration and maintenance services for Hanford Site contractors. The project calibrates and maintains radiation protection instrumentation that is used to ensure personnel safety in the Hanford workplace. Effective CY 2000, the project also calibrates and maintains measuring and test equipment that is used for occupational protection and for research projects on the Hanford Site. Specific tasks performed under this program during CY 2000 included calibration, maintenance, and repair of instrumentation; procurement and testing of new radiological control instruments; administration and technical support of the Hanford Instrument Evaluation Committee (HIEC); and maintenance of a pool of portable survey instruments available for use by site contractors.

The operation of a complete radiation protection instrument calibration and maintenance program is an integral part of the Hanford Site Radiological Control Program. During CY 2000, IS&TP continued to provide complete instrument services including calibration, maintenance, repair, and records management.

Procurement of new instruments is initiated by the site contractors, or jointly by the contractors through the HIEC, and the procurement costs are charged to the contractor using the instruments. The Hanford contractors, through the evaluation, calibration, and maintenance programs of IS&TP provide the site with high-quality instrumentation that is reliable, accurate, and capable of performing at the level necessary to ensure personnel safety as required by 10 CFR 835. Calibrations are performed using the mandatory guidance in ANSI N323-1978, *Radiation Protection Instrumentation Test and Calibration* (ANSI 1978). IS&TP activities fall under several basic tasks. These basic tasks are 1) administration of the Hanford Site pool of portable survey instruments; 2) calibration and maintenance of radiation detection instruments; 3) calibration and maintenance of measuring and test equipment; 4) evaluation and publication at Hanford Site of all site portable survey instrument environmental parameters; 5) maintenance of a calibration records database; 6) maintenance of all the necessary radiological, electronic, and mechanical standards traceable to NIST; and 7) administration and technical support of the HIEC. Several of these basic tasks and other important supporting tasks performed in CY 2000 are described in this chapter.

6.1 Routine Operations

Routine operations include instrument pool management, calibration and maintenance services, and calibration record management, as described in the following sections.

6.1.1 Administration of the Portable Instrument Pool

Administration of the portable instrument pool includes maintaining a sufficient inventory of commonly used instruments to ensure that there is a sufficient supply to meet the daily instrumentation

needs of the field organizations. A second aspect of managing the portable instrument pool is identifying and disposing of instruments that should be removed from service.

During CY 2000, 80 Bicron Surveyor X count rate meters with integral scalers were added to the portable instrument pool. The instruments were purchased to meet an increasing demand for portable alpha meters (PAMs) with integral, digital scalers. These instruments are used to meet DOE contamination limits for releasing material to the public.

6.1.2 Calibration and Maintenance Service

During CY 2000, 14,546 calibrations were performed by IS&TP for the Hanford Site. Table 6.1 details the number of instruments calibrated by calibration class and compares the volume with the number of calibrations performed during previous calendar years. Because the measuring and test equipment calibrations were performed by another organization prior to CY 2000, statistics for the Measuring and Test Equipment calibration project (M&TE; discussed below) are not provided for previous years. Tables 6.2 through 6.6 provide additional details about the number of calibrations performed for each prime contractor during CY 2000. Figure 6.1 illustrates the total number of calibrations performed each month for the Hanford Site. The figure is provided because it illustrates the cyclic nature of the calibration volume.

The total number of calibrations performed increased slightly from the 14,200 calibrations performed in CY 1999, which was slightly lower than the previous year. This indicates that the annual calibration volume is leveling off or, perhaps, increasing.

Table 6.1. Instrument Calibrations by Unit-Price Category and by Calendar Year

Calibration Class	Description of Class	Number of Calibrations by Calendar Year			
		CY 1997	CY 1998	CY 1999	CY 2000
CAMs ^(a)	Continuous air monitors	495	458	465	444
Exposure Rate	Exposure or dose rate survey instrument	2,219	1,896	1,808	1,836
Probes	Probe or detector only	3,944	3,670	3,406	3,551
Electronic Dosimeters	Direct reading, electronic dosimeter	804	647	842	969
Mini Scaler ^(a)	Integral meter and detector	265	320	293	130
Air Flow	Air flow measuring devices	NA	NA	NA	352
Meter only	Electronic calibration of meter or readout	3,973	3,558	3,593	3,915
Pencils	Pocket ionization chamber dosimeter	3,946	3,149	2,690	2,501
Smart Probes	Stand-alone calibration of a "smart" detector	487	486	597	485
Sources	Certification of source activity or emission rate	386	324	300	283
Special Calibrations	Complex calibrations charged by the hour	68	112	87	66
M&TE - all others	Measuring and test equipment/non-radiological	NA	NA	NA	14
Total		16,637	14,620	14,173	14,546
(a) CAMs = continuous air monitors NA = not applicable.					

Table 6.2. CY 2000 Calibration Volume for All Hanford Contractors

Calibration Class	Calibrations Completed by Month for CY 2000												
	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec	Total Hanford Units
Exposure Rate	137	125	148	133	160	153	181	127	237	130	125	180	1,836
Mini Scaler	4	17	8	11	10	12	6	5	19	9	21	8	130
Meter	344	297	273	350	309	286	404	343	481	240	261	327	3,915
Electronic Dosimeter	41	50	42	121	60	76	202	60	137	51	73	56	969
Probe	273	280	268	332	264	263	354	286	429	225	271	306	3,551
Smart Probe	55	47	43	59	41	36	26	24	80	27	24	23	485
CAM	13	33	33	46	41	50	51	39	32	27	38	41	444
Pencil	136	203	106	236	380	162	175	202	267	226	278	130	2,501
Source	25	39	28	36	18	8	33	11	30	13	29	13	283
Specials	10	4	2	4	7	1	6	9	8	5	4	6	66
Air Flow	28	23	10	30	23	12	22	21	105	8	38	32	352
M&TE – all others	0	0	0	0	0	0	0	0	0	6	0	8	14
Total	1,066	1,118	961	1,358	1,313	1,059	1,460	1,127	1,825	967	1,162	1,130	14,546

Table 6.3. CY 2000 Calibration Volume for Fluor Hanford, Inc.

Calibration Class	Calibrations Completed by Month for CY 2000												Total FH Units
	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec	
Exposure Rate	82	66	94	90	104	81	117	73	142	77	72	108	1,106
Mini Scaler	3	9	7	9	9	10	5	4	15	8	18	6	103
Meter	183	126	151	220	184	152	213	191	252	140	134	168	2,114
Electronic Dosimeter	32	29	25	74	54	27	132	22	92	49	53	34	623
Probe	182	150	166	245	183	160	217	187	256	123	131	156	2,156
Smart Probe	4	0	2	0	0	0	0	0	0	0	5	0	11
CAM	12	29	29	34	33	41	43	33	23	27	31	37	372
Pencil	78	76	52	235	267	81	59	72	159	72	132	10	1,293
Source	19	39	20	28	16	8	23	6	21	10	26	12	228
Specials	4	1	0	2	1	1	3	7	6	3	1	1	30
Air Flow	28	7	7	4	16	4	7	10	10	2	20	13	128
Total	627	532	553	941	867	565	819	605	976	511	623	545	8,164

Table 6.4. CY 2000 Calibration Volume for CH2M Hill Hanford Group

Calibration Class	Calibrations Completed by Month for CY 2000												
	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec	Total CHG Units
Exposure Rate	19	28	27	13	17	41	20	25	46	23	14	32	305
Mini Scaler	0	3	1	0	0	1	0	0	1	1	3	1	11
Meter	42	48	46	37	63	43	38	28	53	40	42	56	536
Electronic Dosimeter	4	4	1	25	0	0	9	24	45	0	10	6	128
Probe	43	57	50	36	45	49	55	28	54	45	51	49	562
Smart Probe	0	0	0	0	0	0	0	0	0	0	0	0	0
CAM	0	0	0	3	1	0	0	3	4	0	0	0	11
Pencil	39	113	51	1	66	52	95	86	78	65	59	91	796
Source	3	0	4	5	2	0	7	2	8	3	2	0	36
Specials	0	0	0	0	0	0	0	0	0	0	0	0	0
Air Flow	0	16	1	24	6	6	10	7	87	1	10	12	180
Total	150	269	181	144	200	192	234	203	376	178	191	247	2,565

Table 6.5. CY 2000 Calibration Volume for Bechtel Hanford, Inc.

Calibration Class	Calibrations Completed by Month for CY 2000												
	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec	Total BHI Units
Exposure Rate	19	10	9	13	8	20	15	15	33	21	12	20	195
Mini Scaler	0	0	0	0	0	0	0	0	0	0	0	0	0
Meter	67	63	50	61	33	60	51	62	102	41	48	70	708
Electronic Dosimeter	5	8	16	21	6	38	60	14	0	1	9	16	194
Probe	5	7	16	11	7	28	15	19	46	23	18	45	240
Smart Probe	51	47	41	59	41	36	26	24	80	27	19	23	474
CAM	0	0	1	2	1	8	4	1	2	0	1	1	21
Pencil	3	0	1	0	45	6	1	3	19	32	9	2	121
Source	0	0	1	3	0	0	0	3	1	0	1	1	10
Specials	1	0	0	0	0	0	0	0	0	0	0	0	1
Air Flow	0	0	0	1	0	0	0	0	1	0	0	0	2
Total	151	135	135	171	141	196	172	141	284	145	117	178	1,966

Table 6.6. CY 2000 Calibration Volume for PNNL

Calibration Class	Calibrations Completed by Month for CY 2000												
	Jan	Feb	Mar	Apr	May	Jun	Jul	Aug	Sep	Oct	Nov	Dec	Total PNNL Units
Exposure Rate	17	21	18	17	31	11	29	14	16	9	27	20	230
Mini Scaler	1	5	0	2	1	1	1	1	3	0	0	1	16
Meter	52	60	26	32	29	31	102	62	74	19	37	33	557
Electronic Dosimeter	0	9	0	1	0	11	1	0	0	1	1	0	24
Probe	43	66	36	40	29	26	67	52	73	34	71	56	593
Smart Probe	0	0	0	0	0	0	0	0	0	0	0	0	0
CAM	1	4	3	7	6	1	4	2	3	0	6	3	40
Pencil	16	14	2	0	2	23	20	41	11	57	78	27	291
Source	3	0	3	0	0	0	3	0	0	0	0	0	9
Specials	5	3	2	2	6	0	3	2	2	2	3	5	35
Air Flow	0	0	2	1	1	2	5	4	7	5	8	7	42
M&TE – all others	0	0	0	0	0	0	0	0	0	6	0	8	14
Total	138	182	92	102	105	106	235	178	189	133	231	160	1,851

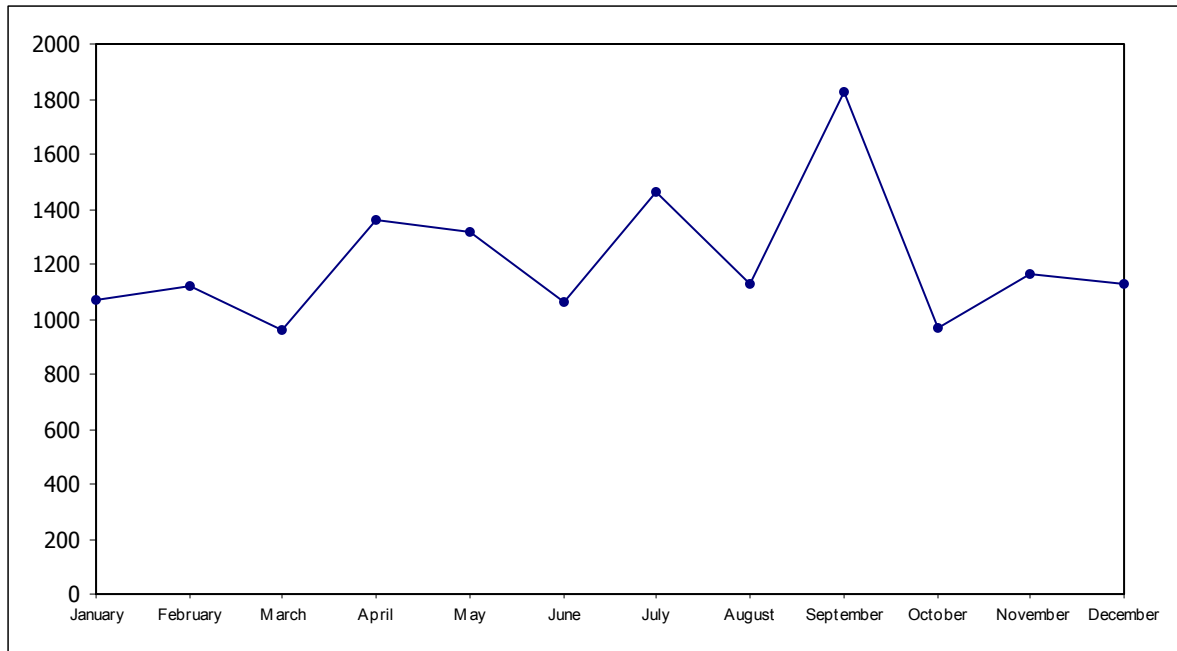


Figure 6.1. Total Number of Calibrations for Hanford Clients During CY 2000

During CY 2000, IS&TP assumed responsibility for managing the PNNL M&TE. The project was previously managed by the Facilities and Operations organization. Because both projects require similar infrastructures, and because IS&TP has a well-developed, mature process for managing calibration projects, the M&TE function was moved into IS&TP. The result is that IS&TP now offers calibration services for other types of equipment besides just radiation detection instrumentation.

6.1.3 Calibration As-Founds Out-of-Tolerance

Part of the calibration service provided by IS&TP is quantifying the as-found condition of each instrument when it is returned for calibration. The as-found condition is typically documented as the instrument's response to the calibration standards and is recorded before any adjustments are made to the instrument's response.

A total of 102 instruments calibrated during CY 2000 were found to be significantly out of tolerance when returned for calibration (that is, the instrument's response was not within $\pm 20\%$ of the conventionally true value of the calibration field). The number of out-of-tolerance notifications issued is consistent with previous years (last year's total was 101 notices). This is an indication that the instruments in the portable instrument pool are not aging to the point of being unreliable.

The total does not include instruments that were returned for calibration with flaws or defects that would render the instrument obviously unusable to the user. Nor does it include instruments

that were repaired prior to calibration because any repairs would invalidate the as-found readings. In each case, the organization that used the instrument was notified of the out-of-tolerance condition.

When a single instrument model seems to have a large number of calibration as-founds that are out of tolerance, a detailed review of all calibration as-founds for that instrument model is conducted. If more than 15% of the instruments returned for calibration have as-founds out of tolerance, the calibration interval for that instrument model is shortened. During CY 2000, as-found data for several instrument models were investigated for adverse trends. The models investigated were the Nuclear Research Corporation AN/PDR-70 “Snoopy”; the Eberline Model 3, 4, and 5-series Alpha continuous air monitors (CAMs); the Eberline GM count rate meters; and the Eberline RO-3B “CP.” The as-found data for all models were acceptable, and none of the calibration intervals were adjusted.

6.1.4 Maintenance of the Calibration Records

IS&TP manages the calibration records for all instruments, sources, and dosimeters calibrated by IS&TP. The records are scanned to allow for ready retrieval before being sent to record storage. Upon request, copies of calibration records are provided to customers.

6.2 Program Improvements in Calibration and Maintenance Operations

During CY 2000, IS&TP radiological calibration project merged with the Facility and Operations M&TE calibration project. The consolidation allows both projects—radiological calibrations and M&TE calibrations—to use the same infrastructure. The end result is reduced cost to the customer because infrastructure costs (calibration recall system, database maintenance, records management) are spread across a larger number of calibrations.

6.3 Hanford Instrument Evaluation Committee

The HIEC was established to provide a Hanford intercontractor information exchange mechanism to ensure that the highest-quality portable and semi-portable radiological protection instrumentation program is maintained at Hanford. The responsibilities of the committee include the following:

- Discuss and propose solutions to ongoing or potential radiological instrumentation problems and needs onsite.
- Identify new radiological instrumentation available from manufacturers that may be useful to Hanford Site operations.
- Oversee the procurement of the instruments and review the evaluations of the performance by contractor organizations.

- Establish or review minimum acceptable operational criteria for portable and semi-portable radiological instrumentation used for safety on the Hanford Site.
- Promote information exchange between contractors on radiological protection instrumentation usage and problems/resolutions.

Representatives from all of the Hanford contractors and a representative of RL are on this committee.

During CY 2000, the HIEC continued to evaluate instruments identified as needing further evaluations before being approved and placed on the “approved instrument list.” The HIEC maintains the “approved instrument list” as a mechanism to demonstrate compliance with the 10 CFR 835 requirement that instruments “shall be appropriate for their environment.”

IS&TP supports the HIEC by serving as the organization’s secretary and providing administrative and technical support. In this role, IS&TP maintains the approved instrument list and the record files of all instrument evaluations completed for Hanford Site customers. IS&TP also provides technical support in the areas of instrument testing and design.

During CY 2000, IS&TP began issuing HIEC meeting minutes as electronic documents accessible through the calibration web page. This reduced the effort required to distribute minutes and improved the availability of HIEC historical documents to Hanford technical staff.

6.4 Supporting Technical Studies

No technical studies were performed under this project during CY 2000.

6.5 Program-Related Professional Activities

Staff presentations and external professional activities during CY 2000 are listed in this section.

6.5.1 Presentations

Johnson, M. L., *Evaluation of the MGP Instruments Model DMC 2000S Electronic Dosimeter*, presented at the MGP Instruments, Inc., User’s Group Meeting, Atlanta, Georgia, June 2000.

6.5.2 External Professional Activities

Bratvold, T. E., Member of the Health Physics Laboratory Accreditation Assessment Committee.

Johnson, M. L., Co-Chairperson of the Working Group for ANSI N323C, *Radiation Protection Instrumentation Test and Calibration—Air Monitoring Instruments*.

Johnson, M. L., Member of the Working Group for ANSI N323A, *Radiation Protection Instrumentation and Calibration—General Requirements and Portable Instruments*.

Johnson, M. L., Member of the Working Group for ANSI N323D, *Radiation Protection Instrumentation and Calibration—Fixed Instruments*.

7.0 Radiation Standards and Calibrations Program

The primary function of the Radiation Standards and Calibrations Program (RS&CP) is to maintain the necessary radiological reference fields to facilitate appropriate characterizations and calibrations within the Hanford IS&TP and HEDP. In support of this task, special instrument and dosimeter response-characterizing equipment and supplemental radiological reference fields are maintained, as necessary. This activity provides the means to characterize instrument and dosimeter response to various radiation fields encountered at Hanford and to ensure that calibration capabilities are available in accordance with recommended standards and guides. The RS&CP is coordinated by the Calibration Research and Accreditation (CR&A) subgroup of the DR&T technical group. This group also supports other Hanford entities as well as DOE-HQ, other departments of the U.S. Government, and the private sector within its NVLAP scope of accreditation as a Calibration Laboratory for Ionizing Radiation, which has been maintained since 1994. Standards and methodologies developed in support of non-Hanford applications serve to enhance the capabilities available to the Hanford Site. Typical project activities include the following:

- providing a pathway of traceability for the calibration sources to the NIST
- maintaining radioactive sources, X-ray-generating devices, and instruments that serve as radiological standards
- reviewing calibration standards, regulations, and handbooks to ensure that calibration and characterization protocols agree with technically accepted methods.

Program activities conducted during CY 2000 are discussed in the following sections.

7.1 Routine Operations

Routine activities conducted by program personnel included maintenance of radiological standards, including reference class instruments and reference fields traceable to national standards, and the development of new and/or specialized capabilities. These existing and new capabilities support a variety of applications at the Hanford Site, within the DOE and other U.S. Government communities, and throughout the international radiological protection industry, in both the private sector and government programs. The activities related to radiological standards and capabilities and applications are discussed in the following sections.

7.1.1 Standards and Capabilities

The radiological reference fields maintained include gamma, beta, and neutron isotopic sources and X-ray-generating devices. These standards and capabilities are configured to deliver well-characterized and reproducible quantities of radiation dose or exposure to environmental or personnel dosimeters, radiological survey instruments, etc., for providing NIST-traceable calibration and/or response

characterization. In addition, reference-class instrumentation is maintained for the purpose of calibration, characterization, constancy verification, and traceability transfer.

Gamma Ray Reference Fields

Available photon sources include various activities of ^{137}Cs and ^{60}Co configured in either collimated-beam, well, or open-field geometries, and an ^{241}Am source configured for irradiation in a 2π geometry, as listed in Table 7.1. These sources are located in the 318 Building. The “open” sources listed in Table 7.1

Table 7.1. Available Gamma-Ray Sources (1999)

Source	Geometry	Nominal Rate/Range ^(a) (R[rem]/hr)	Location in 318 Bldg. (Room)	Reference No.	Primary Photon Energy (MeV)
^{60}Co	Open (4π)	0.6 / 2	106	318-164	1.17/1.33
	Beam ^(b)	0.18 – 88 ^(c) 2 – 1000 ^(d)	8	318-037	
	Beam ^(e)	2 – 750 ^(c) 26 – 8500 ^(d)	8	318-036	
	Beam	11.8 – 3700 ^(c) 135 – 42500 ^(d)	8	318-353	
^{137}Cs	Well	10^{-4} – 0.007 ^(c) 0.001 – 0.130 ^(d)	121	318-031	0.662
	Well	0.025 – 2.700	121	318-030	
	Well	0.004 – 1.3 ^(c) 0.065 – 22.0 ^(d)	121	318-288	
	Beam	.001 – 0.25 ^(c) 0.070 – 24.0 ^(d)	8	318-040	
	Open (4π)	0.34 / 1.3	106	318-001	
	Beam	0.008 – 2.5 ^(c) 0.7 – 240 ^(d)	8	318-044	
	Open (4π)	1.8 / 6.8	106	318-029	
	Beam	2.3 / 21	6	318-131	
^{241}Am	Open (2π)	0.125	6	318-184	0.060
<p>(a) Values separated by “/” indicate discrete calibration points. Values separated by “–” indicate inclusive range of calibrated rates.</p> <p>(b) Source removed from irradiator system September 1999.</p> <p>(c) Attenuated (Pb).</p> <p>(d) Unattenuated.</p> <p>(e) Source installed into irradiator system September 1999.</p>					

are placed at one of two positions within the facility via a pneumatic air-transfer system. Exposure rates at two discrete distances from the source are typically characterized, but rates at other distances may be derived. “Beam” sources, with the exception of source 318-131, provide a continuum of exposure rates via use of an artifact positioning stand located on a sliding-rail system. Source 318-131 also includes a moveable stand, but it is typically characterized and used only at the 1- and 3-m distances. Artifact placement for the most commonly used positions within these beam irradiation facilities is enhanced by laser alignment capabilities. “Well” sources also provide a continuum of exposure rates and facilitate instrument adjustments during irradiation with minimal exposure to personnel. The source-to-artifact distance is controlled by moving the sources, on a trolley system, up and down within the well via a computer interface.

Gamma reference fields from available ^{137}Cs and ^{60}Co sources are calibrated using reference class ionization chambers equipped with suitable buildup material to establish charged particle equilibrium. The referenced chamber wall depth for such calibrations is typically 726 mg/cm^2 . This depth has been judged suitable based on the typical inventory of instruments calibrated by the IS&TP. This choice of buildup depth is of importance in the case of the “well” geometry sources, in which the scattered radiation may produce non-linear effects for selected instruments. Ionization chambers with significantly less wall material or certain Geiger-Müller (GM) or scintillation devices may display properties of heightened energy dependence.

In addition to the sources listed above, a Nordion Model GB650 “high-intensity” gamma irradiator is available in the 331 Building; it produces high-energy gamma fields from ^{60}Co . This facility uses 12 sources that can be placed in a variety of geometries within tubes set in a circular pattern (see Figure 7.1). The exposure rate is adjusted by selecting a particular source or combination of sources and the specific orientation of the irradiation tube(s) in proximity to the item being irradiated. The range of available exposure rates extends from 7 to 10^6 R/h and has been applied to ultra high-range instrument calibration/characterization, as well as evaluations of radiation fatigue for materials and components. The calibration of this facility is maintained traceable to the NIST through the use of reference standards and methods identical to those used for the 318 Building sources, as described elsewhere in this report. In addition, radiochromic QC dosimeters are provided, where necessary, for establishing a dose gradient within a sample volume or for confirming delivered dose within an irradiated artifact.

X-Ray Photon Sources

A Pantak Model HS320/Series II and two identical Philips Model-324 tungsten-target X-ray machines are currently used by the RS&CP. One Philips machine and the Pantak system are used to produce Bremsstrahlung photon spectra (e.g., NIST techniques M30, S60, M150, H150, and International Standards Organization (ISO) techniques NS150, HK100, etc.), while the second is configured for K-fluorescence technique (narrow) secondary photon spectra (e.g., ISO 4037 techniques F-Mo [17.5 keV], F-Cs [31.0 keV], F-W [59.0 keV], etc., [ISO 1996a; 1996b]) within a shielded enclosure. These reference fields are used for characterization of dosimeter or instrument photon energy dependence in the general region of 10 to 250 keV. The NIST techniques are titled based on the characteristics of the filters used to modify the primary X-ray beam, where “M,” “H,” and “S” indicate moderate, heavy, and special filters, respectively. In general, M and S techniques are characterized by broader spectra and consequently lower

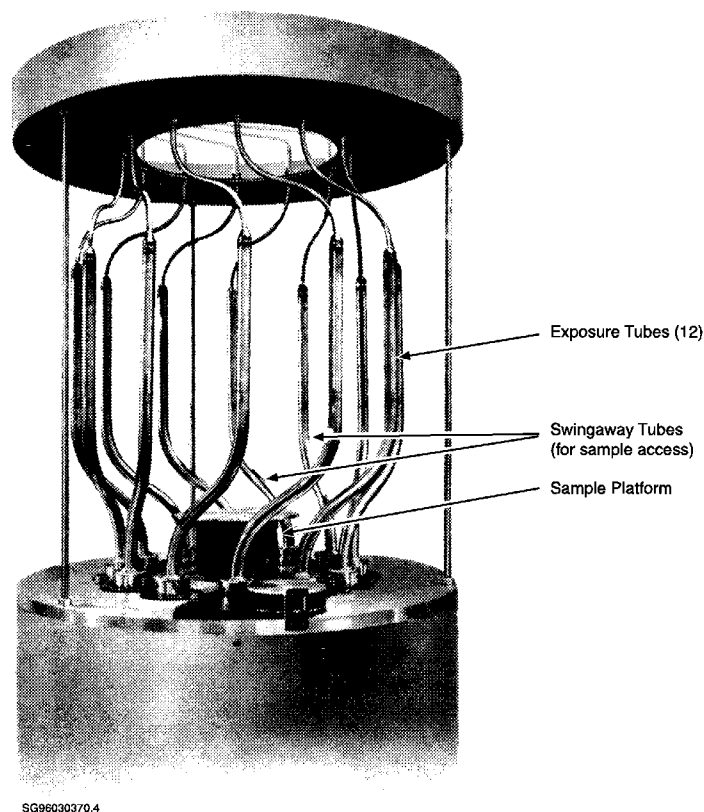


Figure 7.1. GB650 ^{60}Co Irradiator

homogeneity coefficients. The average energy listed for such techniques is only a rough indicator of the beam energy. H technique spectra are typically narrower and their energy can be described more readily as an effective photon energy (i.e., compared with a gamma source with a photon energy of the same half-value layer). As such, they are well suited, and recommended by NIST, for evaluations of dosimeter or instrument photon energy dependence. The ISO techniques titled “NS” are characterized by narrow spectra, while “HK” techniques are generally characterized by broader spectra. K-fluorescence techniques have highly discrete peak energies and are also well suited for energy characterization studies, although the maximum energy currently available is 59 keV.

Figure 7.2 shows an example of several X-ray techniques that have a similar quoted average or effective energy. Tables 7.2a to 7.2c, provide a complete list of currently available techniques, their characteristics or production methods, and the nominal exposure rates available. All of these systems are equipped with laser alignment capabilities to aid in detector/dosimeter positioning.

Neutron Sources

Two configurations of ^{252}Cf neutron sources are available. One configuration allows for the use of available sources within a pneumatic transfer system in the 318 Building Low-Scatter Room (LSR). During use, these sources are placed near the geometric center of a room 10 m wide, 14 m long, and

p y p
Bremsstrahlung vs. K-Fluorescence

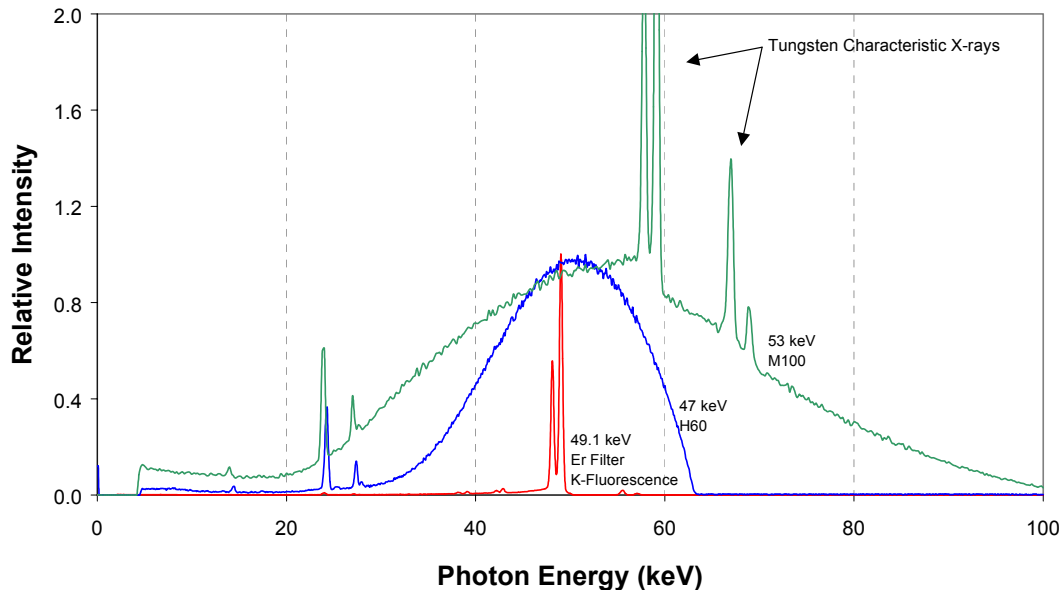


Figure 7.2. Example Spectrum of X-Ray Configurations (peak or average energy normalized to 1.0)

8.8 m high. Such placement minimizes scattered neutrons from the walls, floor, and ceiling at the point of the detector and facilitates the quantification of scatter influence upon the detection device. Sources may be used bare or moderated by a sphere of deuterated water (D_2O) 15 cm in radius, enclosed within a thin stainless steel shell, and covered by 0.051 cm of cadmium. These provide neutron fields that are useful for instrument calibrations as well as for dosimeter characterization in accordance with the specifications of DOE/EH-0027, the *Department of Energy Standard for the Performance Testing of Personnel Dosimetry Systems* (DOE 1986b); HPS N13.11, *Personnel Dosimetry Performance – Criteria for Testing* (ANSI/HPS 1993); and ISO 8529, *Neutron Reference Radiations for Calibrating Neutron-Measuring Devices Used for Radiation Protection Purposes and for Determining their Response as a Function of Neutron Energy* (ISO 1989). In addition, a D_2O -moderator sphere, similar to the one described above, is available without the shell of cadmium. This sphere, while originally intended as a backup, has been used, upon request, to provide neutron test fields with a larger component of thermal neutrons.

The second configuration involves a ^{252}Cf source placed in a well to facilitate easy access for instrument calibration. This source provides a fission spectrum that is significantly altered by the scattering from the concrete sides of the well; however, its calibration is established such that instrument calibrations will be referenceable to bare ^{252}Cf under free-field conditions, for selected instruments.

Table 7.2a. Available NIST-Specified Bremsstrahlung X-Ray Reference Fields (2000)

Technique	Nominal					
	Average ^(a) Energy (keV)	Effective ^(b) Energy (keV)	Half-Value Layer ^(c) (mm Al)	Homogeneity Coefficient ^(c,d) (Al)	Minimum ^(e) Exposure Rate (R/h)	Maximum ^(f) Exposure Rate (R/h)
M20	14		0.15*	69*	3.4	61 (2)
M30	20		0.36*	65*	2.9	134 (5)
M50	29		1.02*	66*	3.5	67 (2)
M60	35		1.68	66	3.2	60 (2)
M100	53		5.02	73	2.8	57 (2)
M150	73		10.2	87	3.7	564 (15)
M200	100		14.9	95	4.4	44 (1)
S60	38		2.77	72	1.2	57 (5)
S75	40		1.86*	63*	4.5	87 (2)
H40	33		2.90*	90*	0.02	4.9 (20)
H50		38	4.2	92	0.05	10 (20)
H60		46	6.0	94	0.07	13 (20)
H100		80	13.5	1.00	0.02	3.0 (20)
H150		120	17.0	1.00	0.10	15 (15)
H200		166	19.8	100	0.09	9.4 (10)
H250		211	22.0	100	0.09	8.7 (10)
H300		251	23.0	99	0.06	5.8 (10)
(a) Average energy is quoted for broad spectra techniques and represents only an approximate indication of the energy. (b) The effective energy is shown for those beam codes for which it is believed to be a meaningful characterization of the beam quality. (c) Values accompanied by “*” are quoted at distance of 50 cm. All others quoted at 100 cm. (d) The homogeneity coefficient is taken as $100 * (1^{\text{st}} \text{ HVL} / [2^{\text{nd}} \text{ HVL} - 1^{\text{st}} \text{ HVL}])$. (e) Quoted at distance of 100 cm and beam current of 0.1 mA. (f) Quoted at a distance of 100 cm and the highest beam current (mA) for which calibration is performed. (Current listed in parenthesis)						

Beta Particle Sources

Beta particle sources (e.g., ^{147}Pm , ^{204}Tl , and $^{90}\text{Sr}/^{90}\text{Y}$) are maintained for dosimetry and instrument characterization. Available sources are listed in Table 7.3 and include those manufactured by Amersham-Buchler, which are calibrated directly by the Physikalisch-Technische Bundesanstalt (PTB), Germany’s national physical standards organization, and those manufactured in the United States by Amersham and Isotope Products Laboratory. Measurements have been made of most “point” geometry sources to verify satisfactory compliance with HPS N13.11 (ANSI/HPS 1993); DOE/EH-0027 (DOE 1986b); and ISO 6980, *Reference Beta Radiations for Calibrating Dosimeters and Dose Rate Meters and for Determining their Response as a Function of Beta Radiation Energy* (ISO 1984), as applicable.

Table 7.2b. Available ISO-Specified Bremsstrahlung X-Ray Reference Fields (2000)

Technique	Nominal					
	Energy (keV)		Half-Value Layer (mm)	Homogeneity Coefficient ^(c)	Minimum Exposure Rate (R/h) ^(d)	Maximum Exposure Rate (R/h) ^(e)
	Average ^(a)	Resolution ^(b)				
Narrow Series						
NS 150	118	37	2.36 ^(f)	96 ^(f)	0.13	25 (20)
NS 250	208	28	5.19 ^(f)	99 ^(f)	0.06	5.4 (10)
High Air Kerma Rate Series						
HK 60	37.3	(h)	2.42 ^(g)	74 ^(g)	1.3	65 (5)
HK 100	57.4		6.56 ^(g)	81 ^(g)	1.7	86 (5)
HK 250	122		16.6 ^(g)	96 ^(g)	5.7	118 (2)
(a) For broad spectra techniques (i.e., HK), average energy represents only an approximate indication of the energy.						
(b) FWHM ($\hat{I} \text{ E/E} \times 100$, where $\hat{I} \text{ E}$ represents the spectrum width corresponding to half the maximum ordinate of the spectrum).						
(c) The homogeneity coefficient is taken as the $100 \times (1^{\text{st}} \text{ HVL} / [2^{\text{nd}} \text{ HVL} - 1^{\text{st}} \text{ HVL}])$.						
(d) Quoted at distance of 100 cm and beam current of 0.1 mA.						
(e) Quoted at a distance of 100 cm and the highest beam current (mA) for which calibration is performed. (Current listed in parenthesis)						
(f) Narrow series techniques quoted in Cu.						
(g) High air kerma rate series techniques quoted in Al.						
(h) Not specified.						

Table 7.2c. Available K-Fluorescence Reference X-Ray Fields (2000)

Technique ^(a)	Peak Energy (keV) ^(a)	Production Method				Exposure Rate (R/hr) ^(b,c)	
		Pre-Filter (Al mg/cm ²)	Radiator/Attenuator	Filter	kVcp	Minimum	Maximum
F-Zn	8.6	0.135	Zinc	NA ^(d)	50	0.04	5.5
F-Zr	15.8	0.27	Zirconium	SrCO ₃	80	0.01	2.1
F-Mo	17.5	0.27	Molybdenum	Zr	80	0.02	2.3
F-Sn	25.3	0.27	Tin	Ag	100	0.02	3.0
F-Cs	31.0	0.27	Cesium	TeO ₂	100	0.01	1.4
F-Nd	37.4	0.27	Neodymium	Ce	110	(e)	(e)
F-Sm	40.1	0.27	Samarium	CeO ₂	120	0.01	1.4
F-Er	49.1	0.27	Erbium	Gd	120	0.005	0.8
F-W _c	59.3	0.27	Tungsten	Yb ₂ O ₃	170	0.006	0.9
F-W _m	59.3	0.27	Tungsten	Yb	170	0.006	0.9
<p>(a) As identified by ISO/DIS 4037-3:1996. Subscripts on F-W Techniques differentiate between filters made of chemical compound (c) and pure metal (m).</p> <p>(b) Nominal.</p> <p>(c) Minimum/maximum estimated at 0.1/15.0 mA.</p> <p>(d) NA = not applicable.</p> <p>(e) Out of service in CY 2000.</p>							

Table 7.3. Available Beta Reference Fields (2000)

Geometry	Isotope (Source No.)	Window Material and Areal Density (mg/cm ²)	Protective Coating Material and Areal Density (mg/cm ²)	Residual Maximum Energy -E _{res} (MeV) (M-Measured, T-Theoretical)	Absorbed Dose Rate ^(a) (rad/h) (Calibration Distance (cm))
Point	¹⁴⁷ Pm (318-290)	Not available	Titanium (2.3)	0.1504 ^(b) (M)	0.05 ^(b) (20)
	²⁰⁴ Tl (318-109)	Silver (20)	Gold (5)	0.53 ^(b) ≤ E _{res} ≤ 0.76 ^(b) (T)	0.005 ^(b) (30)
	²⁰⁴ Tl (318-192)	Glass (6.6)	Kapton (~0.8)	0.608 ^(b) (M)	0.7 ^(b) (35)
	²⁰⁴ Tl (318-360)	Acrylic (0.2)	Kapton (9)	0.557 ^(b) (M)	1.5 ^(b) (35) 2.4 ^(c) (35)
	⁸⁵ Kr (318-009)	Not available	Not available	Not available	2.7 (50)
	⁹⁰ Sr ⁹⁰ Y (318-013)	Silver (50)	Stainless Steel (~75)	1.80 ^(b) ≤ E _{res} ≤ 2.274 ^(b) (T)	0.48 ^(b) (30)
	⁹⁰ Sr ⁹⁰ Y (318-102)	Titanium (100)	Aluminum (20)	1.80 ^(b) ≤ E _{res} ≤ 2.274 ^(b) (T)	0.44 ^(c) (35)
	⁹⁰ Sr ⁹⁰ Y (318-012)	Silver (50)	Stainless Steel (~75)	2.046 (M)	19 (30)
	⁹⁰ Sr ⁹⁰ Y (318-103)	Titanium (100)	Not available	2.085 (M)	13 (35)
Distributed	¹⁴ C (318-032)	Not available	PMMA ^(d)	Has not been measured for these sources.	2.2 (0.2)
	¹⁴⁷ Pm (318-113)	Not available	Kapton (1.5)		0.28 - 0.005 (0.2 -15)
	²⁰⁴ Tl (318-128)	Not available	Kapton (9.5)		0.60 - 0.02 (0.2 - 30)
	⁹⁰ Sr ⁹⁰ Y (318-129)	Not available	Kapton (23.5)		4.09 - 0.16 (0.2 - 30)
	¹⁰⁶ Ru/ ¹⁰⁶ Rh (318-130)	Not available	Kapton (30.7)		<0.01 (0.2)
	Depleted Uranium (318-166)	Not available	Aluminized Mylar (7)		0.204 (0.15)
(a) Nominal at 7 mg/cm ² as of mid-year (2000)					
(b) Quoted with use of flattening filter					
(c) Quoted without use of flattening filter					
(d) The source is polymerized with the Polymethylemethacrylate. Sheet thickness is approximately 1 mm with activity uniformly distributed throughout.					

7.1.2 Traceability to National Standards

Maintaining radiological reference fields traceable to national standards is one of the primary goals of this program. Because the method of traceability is often unclear and periodically evolves, the current pathway for PNNL radiological reference fields is provided here.

Philosophy

Traceability to national standards infers an assurance that calibration fields are established and used in a manner that is consistent with those standards. There are two accepted types of consistency measurements that are commonly used to infer traceability: 1) implied consistency, which is established through the use of a laboratory standard submitted to NIST for calibration within radiation fields applicable to the laboratory; and 2) demonstrated consistency, which can be established through an measurement quality assurance (MQA) interaction with NIST. This latter method is akin to a performance test administered by NIST and is instrumental in verifying measurement traceability, as opposed to simply obtaining or maintaining a traceable source or reference instrument. A disadvantage of traceability based only upon implied consistency is the lack of demonstration to indicate that measurements made of traceable sources or using reference instruments are consistent with those made of or using national standards. Traceability

based upon demonstrated consistency provides the assurance that traceable instruments and/or sources are being used properly (whether to calibrate additional sources [or reference fields] or laboratory instrument standards), so that traceability is appropriately extended as desired.

NIST supports the use of both techniques in maintaining traceability, but favors the practice of performing MQA interactions on a routine basis coupled with providing infrequent instrument or source calibrations. The RS&CP mirrors the NIST philosophy where possible; however, there are some limitations of the NIST capability that require a variance in the normal process. The following sections describe the traceability pathway for each of the radiation types applicable within this project.

Photon Standards

Photon sources (i.e., gamma sources and X-ray techniques) are maintained traceable via both implied and demonstrated consistency verifications. On an as-needed basis, one or more selected laboratory standards (air-equivalent ionization chambers [AICs]) are submitted to NIST for calibration to specific radiation fields. Through CY 2000, six commonly used AICs had been submitted for calibration to ^{137}Cs , ^{60}Co , and many of the available NIST and ISO X-ray techniques, including all but one (M20) of the Bremsstrahlung techniques listed in Table 7.2a. In calibrating these instruments directly to NIST “primary standard” reference fields, they are deemed “secondary standards” and are used in the process of calibrating other radiological reference fields and/or reference instruments for use as tertiary or working standards. The most current representation of the traceability pathway is depicted in Figure 7.3. In some cases, secondary standard instruments have been used to calibrate or verify the constancy of working standard radiation fields such as the well calibrators. This practice is acceptable but avoided whenever practical, because it exposes the valuable secondary standards to increased use and the potential for damage.

To achieve demonstrated consistency, NIST has conducted MQA assessments of PNNL photon reference fields since 1984, each time selecting a subset of the available sources and/or X-ray techniques for intercomparison. There were no MQA measurements performed through NIST in CY 2000.

Currently, NIST does not maintain capabilities for K-fluorescence X-ray or ^{241}Am reference fields. Although traceability for these fields has been established using two additional AICs and a pathway similar to that identified in Figure 7.3 for a limited number of fluorescence techniques, the primary reference fields are maintained by the National Radiation Protection Board (NRPB) of the United Kingdom. Traceability for irradiations and calibrations made using these reference fields are implied. The accuracy of these reference fields is confirmed via long-term trending of the transmission chamber output and/or reference standard AIC measurements.

Neutron Standards

Neutron traceability for all irradiations and measurements performed using PNNL sources is currently only implied. The primary pathway to NIST is through direct calibration of PNNL ^{252}Cf sources, in terms of neutron emission rate, within the NIST Manganous Sulfate Bath Facility. Free-field dose-equivalent rates are calculated for these sources in their bare and moderated configuration based on NIST

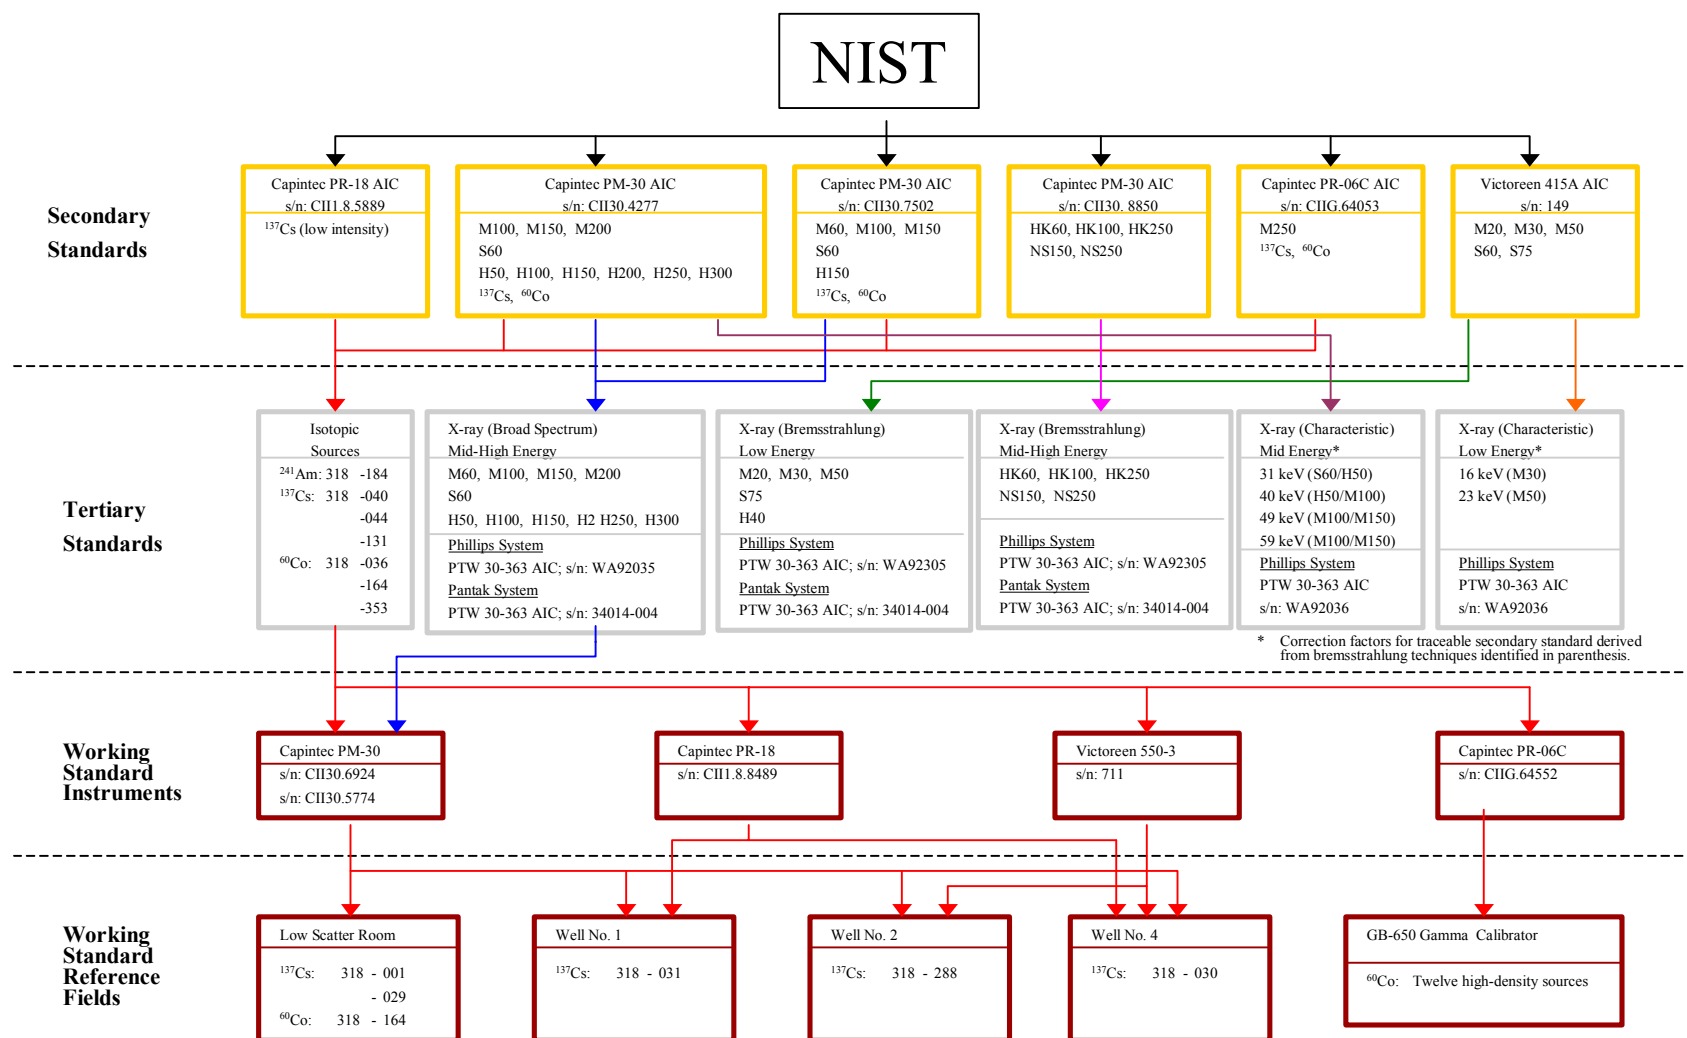


Figure 7.3. Typical Traceability Pathway for PNNL Photon Reference Fields

recommendations provided in the National Bureau of Standards (NBS) Special Publication 633, *Procedures for Calibrating Neutron Personnel Dosimeters* (DOC/NBS 1982). A Nuclear Research Corporation (NRC) Model NP-2 portable neutron monitor (Snoopy) and an Eberline NRD neutron probe are maintained as tertiary standards, which are used to calibrate a well-geometry ^{252}Cf source referenced to free-field conditions. The calibration well is currently established as a working standard specifically for use with these two detector configurations of survey instruments. Use of the well for calibrating any other neutron survey instrument would not necessarily preserve any implied traceability. The traceability pathway for neutrons is shown in Figure 7.4.

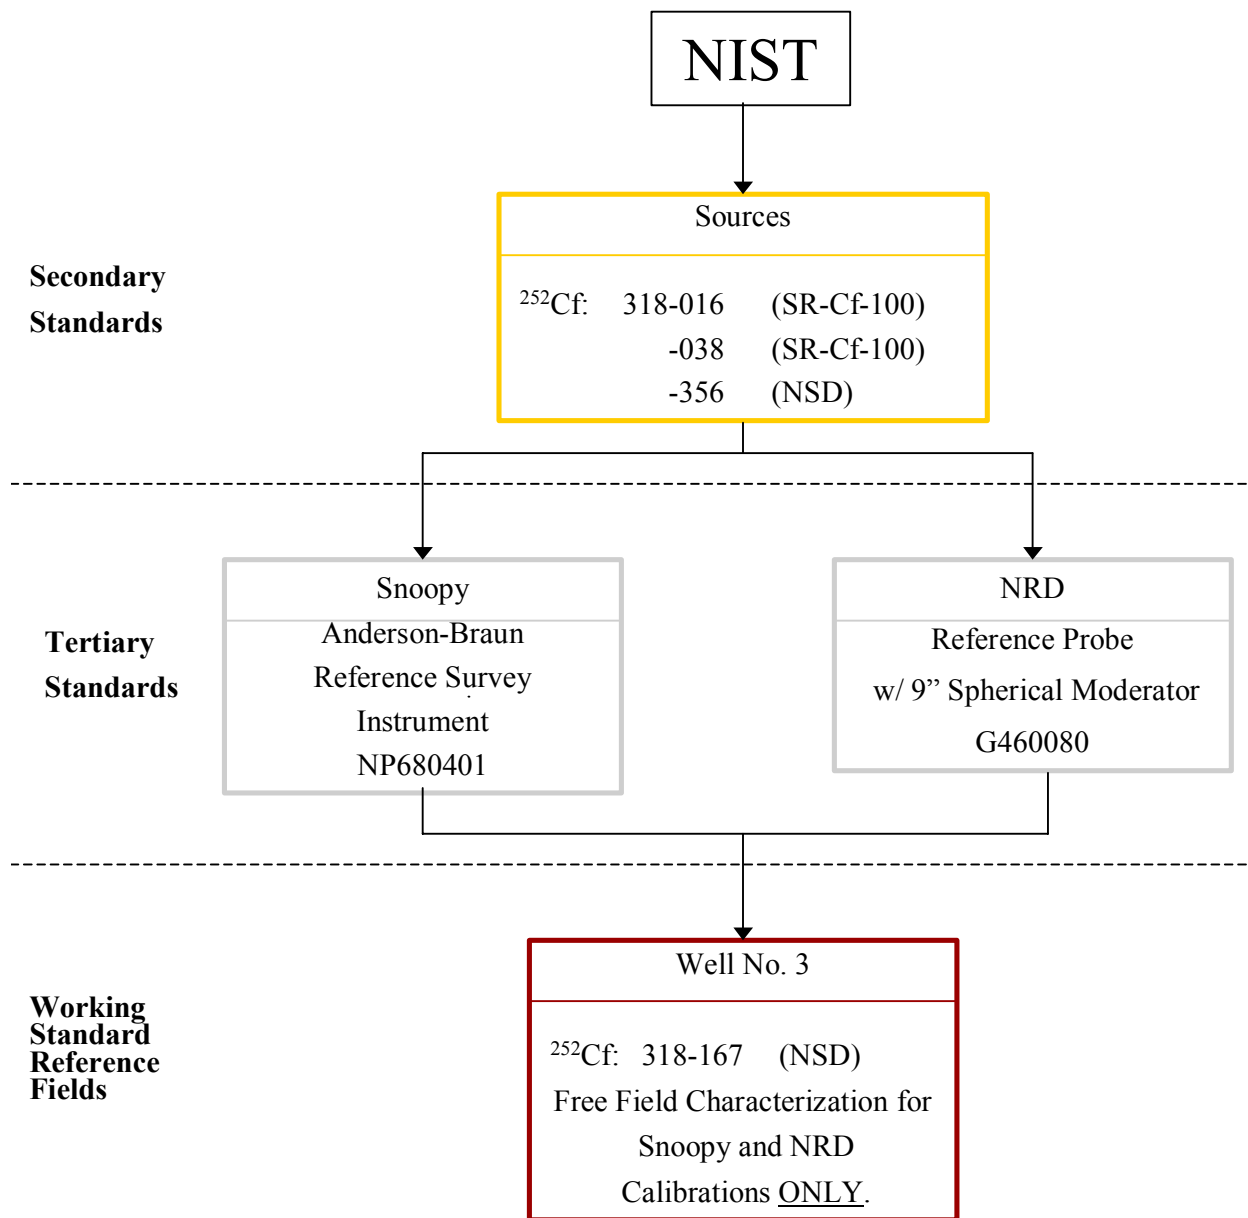


Figure 7.4. Typical Traceability Pathway for PNNL Neutron Reference Fields

MQA interactions are especially desirable for neutron sources as a means to confirm that various parameters are properly determined and/or are accounted for in the use of these sources. Influences such as air scatter, room return (scattered neutrons from walls, ceiling, and floor), source anisotropy, and inherent photon contribution must be properly characterized, either by measurement, calculation, or both. Source aging is a concern due to the magnitude of isotopic contaminants (primarily ^{249}Cf , ^{250}Cf , and ^{251}Cf), which remain following source manufacture and are not directly identifiable via a single NIST calibration. Also, when configured with the D_2O moderating sphere, there are concerns about subtle differences between the NIST design and the PNNL assembly. The NIST design almost completely surrounds the source and is more closely related to the referenced dose equivalent conversion factor, while the PNNL assembly, with an inherent void, allows placement of the sphere around the end tube of the pneumatic transfer system. Monte Carlo modeling suggests that the effect of this void is substantial; however, reliable measurements that can substantiate this model have not been completed. Until measurements confirm or refine the magnitude of this effect, the calculated value will continue to be treated as a component of uncertainty rather than being used as a correction factor applied to the dose equivalent rate.

During the past several years, numerous joint efforts by NIST and PNNL have been conducted to establish a suitable method for neutron MQA intercomparisons in order to demonstrate traceability. These intercomparisons have steadily improved as sources of uncertainty are reduced or better understood; however, there continues to be a bias in intercomparison results induced, in theory, by the acknowledged differences in the PNNL source configurations versus those of NIST. A clear explanation and resolution for the measured bias is not a trivial matter and will continue to be investigated.

Beta Sources

The NIST-traceability of beta reference fields is based upon both implied and demonstrated consistency. Of highest order in the PNNL reference field hierarchy are the PTB sources identified in Section 7.1.1, including $^{90}\text{Sr}/^{90}\text{Y}$ (sources 318-012 and -013) and ^{204}Tl (sources 318-014 and -109). These sources are considered secondary standards because they were initially calibrated and are certified through the PTB and continue to be periodically intercompared with NIST via MQA interactions. The NIST maintains a similar set of sources at its facility that have been characterized/verified both quantitatively and qualitatively.

PNNL maintains a Physikalisch-Technische Werkstätten (PTW) extrapolation ionization chamber for use in performing measurements of absorbed dose rate from the various sources. This chamber is generally considered to be an absolute standard; however, in conforming with the methods used for other radiation fields within the laboratory, it is designated as a tertiary standard. As such, it is the primary link between the PTB sources and all other beta sources.

In many cases, beta irradiations/calibrations are performed using alternate point sources of isotopic distribution similar to the PTB sources, but with subtle differences in construction material and/or activity, including sources 318-102, -103, and -192 (see Table 7.3). The $^{90}\text{Sr}/^{90}\text{Y}$ sources (318-102 and -103) were calibrated directly by NIST (source 318-102 [74 MBq] in 1986 at NIST and source 318-103 [1.85 GBq] at PNNL by a visiting NIST scientist). The latter source was calibrated with PNNL's PTW

extrapolation ionization chamber. Based on the level of these calibrations, source 318-102 is also considered a secondary standard and source 318-103 is relegated to the tertiary level. The traceability pathway for beta reference fields and the extrapolation chamber is shown in Figure 7.5.

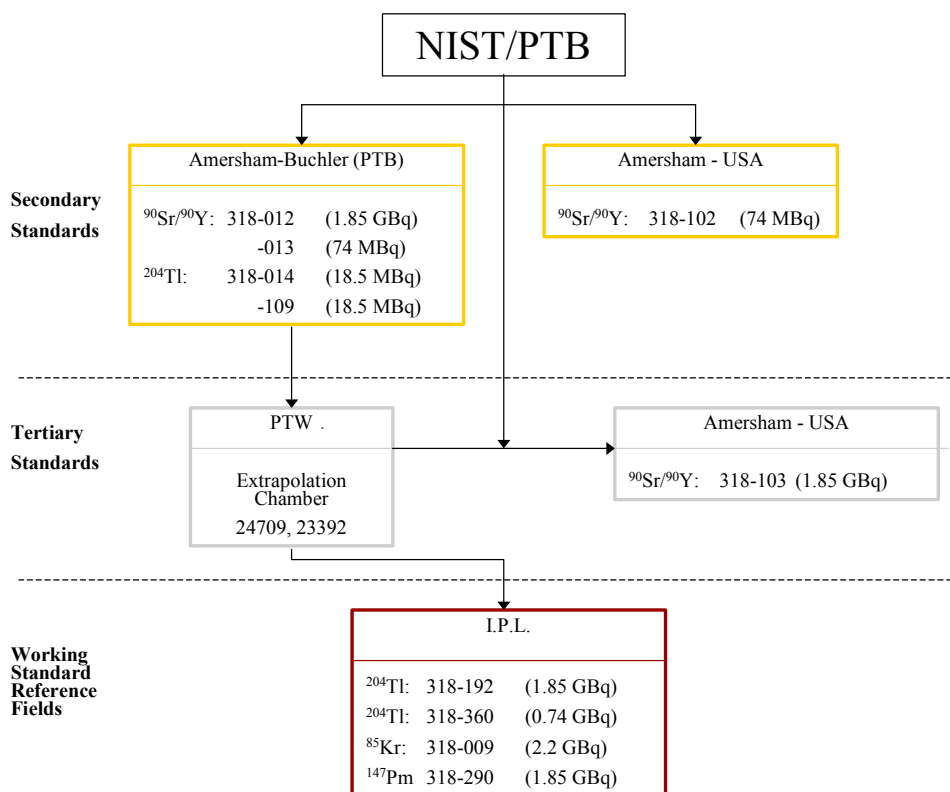


Figure 7.5. Typical Traceability Pathway for PNNL Beta Reference Fields

The periodic MQA intercomparison that NIST conducts with the PNNL calibration laboratory involves the use of a NIST or NIST-approved transfer standard. Intercomparisons with NIST were performed from 1984 to 1985, 1991 to 1992, and in 1999. No beta MQA measurements were performed or initiated during CY 2000.

7.1.3 Quantitative and Qualitative Confirmation of Standards

Radiological reference fields originating from isotopic sources are dynamic in their output due to both the effects of radioactive decay and to the general content of the source material. If the isotopes are generally pure, then changes are typically limited to source decay. If impurities exist or if the decay of the primary isotope results in a radioactive decay product, then changes in the apparent strength and quality of the reference field are more complex. Reference fields generated by X-ray devices may also be dynamic. The eventual degradation of the components of the system may affect the quality and intensity of the primary beam. Furthermore, filters used to condition the useable beam may degrade over time, also potentially altering the radiation quality.

Initial calibrations and characterizations are designed to ensure that PNNL reference fields are adequate and comply with industry standards as identified above. Subsequent measurements are performed at suitable intervals to ensure that source dynamics are as expected. As a minimum, these measurements take into consideration the following criteria for isotopic sources:

- the general content (including possible impurities) of the source material
- the half-life
- the age and/or historical stability
- whether or not an automated positioning system is used to obtain a continuum of exposure/dose equivalent rates and, if so, the stability of such a system
- the stability and/or reproducibility of the source position or positioning system
- the constancy of ambient conditions (e.g., addition of major structures, equipment, or other sources of potential scatter).

For X-ray reference fields, criteria for consideration include the following:

- the constancy/stability of the X-ray equipment
- the quantity of use
- the properties of the materials used within the various beam filters
- the constancy of ambient conditions (e.g., addition of major structures, equipment, or other sources of potential scatter).

Given the above criteria, both the initial and subsequent constancy verification measurements of reference field quantity and quality are typically unique for each capability.

The verifications performed in CY 2000 are summarized in the following sections.

Photon Sources

Well-geometry photon sources were verified during the year using an approach that examines critical exposure rates most commonly used for calibration of detectors and that also assesses the calculational functions of the positioning system in a comprehensive manner. All three systems were found to be consistent with their respective prior calibrations and no complete recalibrations were found to be necessary. However, it was determined that the calibration of Well 1 (318-031) with the attenuator in place, which uses the large-volume PR-18 ion chamber as the reference standard, was inconsistent with practices applied on the other wells. This same condition was identified the prior year and was not

corrected as anticipated. The previous full calibration of this system used a response correction factor established under ideal conditions for the calibration chamber, which has a wall thickness of 212 mg/cm². For other wells, the calibration has been normalized to a buildup thickness of 726 mg/cm² (i.e., that of the PM-30 reference ion chambers), which is more consistent with the normal wall thickness of field detectors calibrated using the wells. Data from the last full calibration of Well 1 (December 1997) were compensated appropriately for this difference and reference fields in the nominal range of 0.1 to 7.0 mR/h were adjusted higher by 4% to 6%.

High-Exposure Facility sources were verified using an approach similar to that used for well-geometry sources. The LSR gamma sources were verified using the new measurement protocol developed in 1998. Other photon isotopic sources (i.e., Shepherd ¹³⁷Cs and ²⁴¹Am irradiators) were verified as in prior years and found to be consistent.

After moving to a 1-year interval for calibration verification on the X-ray system in CY 1999, troubles with the primary Philips X-ray machines during the end of that year ended the use of those particular machines. During the ensuing recovery, a backup Pantak machine was brought online for use with most of the Bremsstrahlung techniques and replacement efforts began for the Philips systems. As a result of this, it was considered prudent to return to a more frequent interval for calibration. X-ray calibrations have also been structured around a moving average of multiple calibrations.

The increased frequency, selected to be 6 months, would also enable a quicker build up of calibration data. This 6-month calibration interval was maintained for each X-ray technique on the Pantak system throughout CY 2000 and will be implemented for the Philips systems, as well, during its continuing return to service. Following several calibration cycles, the interval for X-ray calibrations will again be reviewed and, if warranted, will again be extended to 1 year.

Neutron Sources

Well 3, containing a ²⁵²Cf source (318-167), was calibrated using the NRC Rem-Rad (Snoopy). The mean bias in comparison to the prior calibration in CY 1999 was ! 1.6%. The bias ranged from ! 0.8% to ! 3.2%, but there was no correlation with the position of the source, indicating that there were no problems with the positioning system. It was considered likely that the identified bias was due to a change in the half-life of the source, which is anticipated to have a steadily increasing influence from ²⁵⁰Cf as it ages.

Beta Sources

Beta sources used most commonly for calibration or characterization purposes, ¹⁴⁷Pm source 318-290, ²⁰⁴Tl source 318-192, depleted uranium source 318-166, and ⁹⁰Sr/⁹⁰Y sources 318-102 and -103, were confirmed via extrapolation chamber measurement. Due to the extensive efforts required to perform complete measurements of absorbed dose from beta sources, those used only occasionally are calibrated/confirmed only when needed. All measurements confirmed the previously established dose rates of the sources within the prior measurement uncertainty.

Reference Standard Instruments

Routinely used instrument standards were verified for consistency, as necessary, to ensure their subsequent accuracy for measuring reference fields. These included various AICs used to perform photon reference field measurements, the PTW extrapolation chamber used to assess beta reference fields, and the reference NRC-Snoopy survey instrument used to convey calibration to Well 3.

7.1.4 Applications

The capabilities maintained, in part, via the RS&CP and under the custodianship of the CR&A subgroup can be subdivided into general areas of support for passive and active radiation measurement and dosimetry. These areas are described below.

Traceability Transfer

The radiological reference fields and reference class instruments available within the RS&CP suit the function of establishing or extending traceability to NIST. Most importantly under this project, this applies to the calibration/characterization of working class reference fields such as the well calibrators and panoramic gamma calibration fields available in the 318 Building and the calibration of dosimeter devices used in support of external dosimetry efforts (e.g., calibration/testing of dosimeters, dosimeter readers, and automated dosimeter irradiation devices).

Similar transfers of traceability are available to those outside of the immediate facility as well. These are facilitated by the submission of dosimetry devices or reference instruments for irradiation/calibration within the NIST-traceable reference fields. These irradiations serve to establish implied traceability for the user/owner reference field or dosimetry analysis capabilities.

Traceability Confirmation

The radiological reference fields are used to provide a blind evaluation of performance, either in the area of instrument calibration or external dosimetry analysis. Such MQA tests help ensure that the participant uses NIST-traceable artifacts consistently and, if necessary, appropriately addresses external influences characteristic of related analytical equipment and/or the calibration environment.

Unique Calibration or Investigative Needs

Traceable radiological reference fields may be configured specifically to meet or approximate the needs of a select application for evaluation of field instrument response, reference class instruments, and dosimetry. Historically, reference fields have been structured to account for alternate radiation field geometries, special beta source attenuation configurations, and interpolation of detector response to atypical calibration energies, short-lived nuclides, and mixed fields.

Characterization/Type Testing

Reference fields are used to evaluate lower levels of detection; neutron, beta, and photon energy dependence; the influence of contaminating radiation fields on detectors; response linearity; geometry dependence; and acceptance testing.

CY 2000 Summary

During CY 2000, efforts focused on the above-described scopes of work. Within the scope of traceability transfer, calibration of the various radiological reference fields in the 318 Building were confirmed as described in Section 7.1.3.

In support of traceability confirmation, Hanford dosimeters were exposed on a monthly, quarterly, and annual basis to provide audit and QC evaluations of the PNNL external dosimetry analysis system. In addition, FH contracted for exposed dosimeters on a monthly basis as an independent evaluation of the PNNL external dosimetry analysis system. In all, approximately 1,355 Hanford dosimeters were exposed to controlled doses of radiation for this process.

Characterization and type testing efforts during CY 2000 supported both external dosimetry and instrument calibration efforts. Collectively, approximately 310 dosimeters were exposed to investigate dosimeter configuration and the effects of specific irradiation geometry conditions on the response of Hanford whole body and/or extremity dosimeters. Electronic dosimetry and survey instrument devices were irradiated in support of energy dependence testing and evaluations of sensitivity to beta radiation.

7.2 Operational Improvements

During 2000, operational improvements were made to develop and enhance techniques, systems, and processes, as described in the following sections.

7.2.1 Repair/Replacement of X-Ray Systems

Work continued on implementing the backup, Pantak X-ray system for techniques not configured during the CY 1999 and by early 2000, the full Bremsstrahlung X-ray capability had been restored. Normally, when a move to a secondary system or alternate reference field capability takes place, an intercomparison of that system would be made against the primary fields using typical artifacts calibrated or irradiated using that system. This is desirable to identify whether subtle differences in the systems, which may not be realized by standard characterization methods, might potentially be detectable on such artifacts. Unfortunately, a direct intercomparison with the primary reference fields was not possible due to their catastrophic failure. A review of Hanford dosimeters performed in 1999 was useful in gaining confidence that the new reference fields were performing well; however, more proof was sought to provide additional confidence. That additional confidence was gained via a review of dosimeter test data reported by processors undergoing NVLAP proficiency testing. An evaluation of general performance trends provided objective evidence that X-ray reference fields generated by the backup system were indistinct from those of the primary system.

The repair of the Philips systems continued through September 2000. When complete, the primary X-ray facility was equipped with two new model MCN-323 X-ray tubes, three upgraded generators, and two larger capacity oil coolers. The new Bremsstrahlung system was placed through its basic characterizations, including evaluations of inherent filtration, beam centering, and adequate coverage of a phantom at the standard irradiation distance. Furthermore, each of the available techniques were re-characterized for half-value layer, homogeneity coefficient, spectra, and field non-uniformity as well as the requisite calibration. The fluorescence system was placed through evaluations to ensure proper target focus, followed by spectra and non-uniformity measurements for each technique. During this re-characterization, it was decided to implement the previously unused primary filters. These filters had not been used prior to this because it had been considered to offer little improvement in the spectra at cost of beam intensity (exposure rate). However, during this cycle of measurements, it was found that the rate was not severely impacted except for the lowest energy techniques (see Figure 7.6). However, spectral analysis identified that these same low energy techniques received the most benefit in terms of reducing unwanted low-energy noise (see Figures 7.7a and 7.7b).

The K-fluorescence system was returned to service in September and the primary Bremsstrahlung system was returned to service in October. Both systems were placed on a 6-month re-calibration schedule. The frequency of calibration will be evaluated following at least three calibrations.

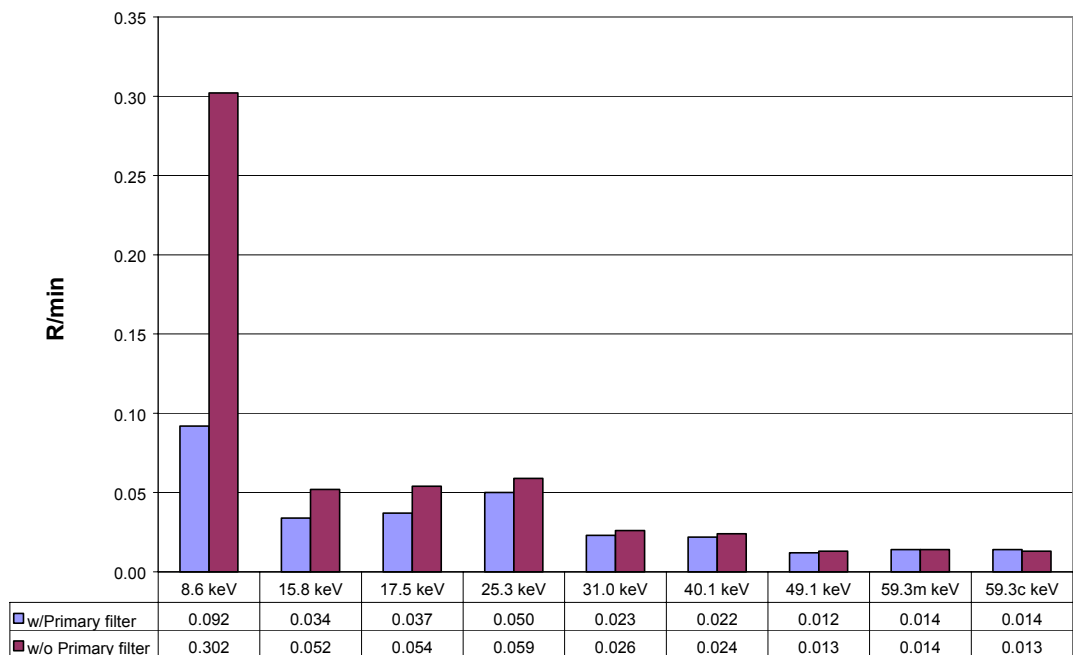


Figure 7.6. Reduction in K-Fluorescence Exposure Rates Due to Addition of Primary Filter (quoted at 15 mA)

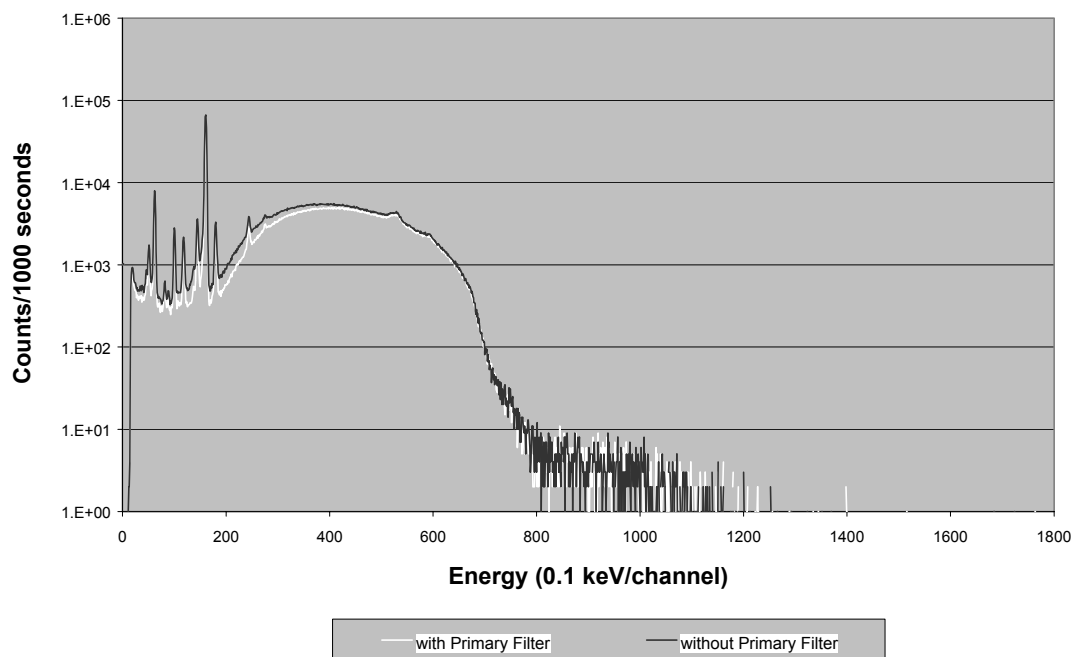


Figure 7.7a. Effect of Primary Filter on 17.5-keV K-Fluorescence Spectra

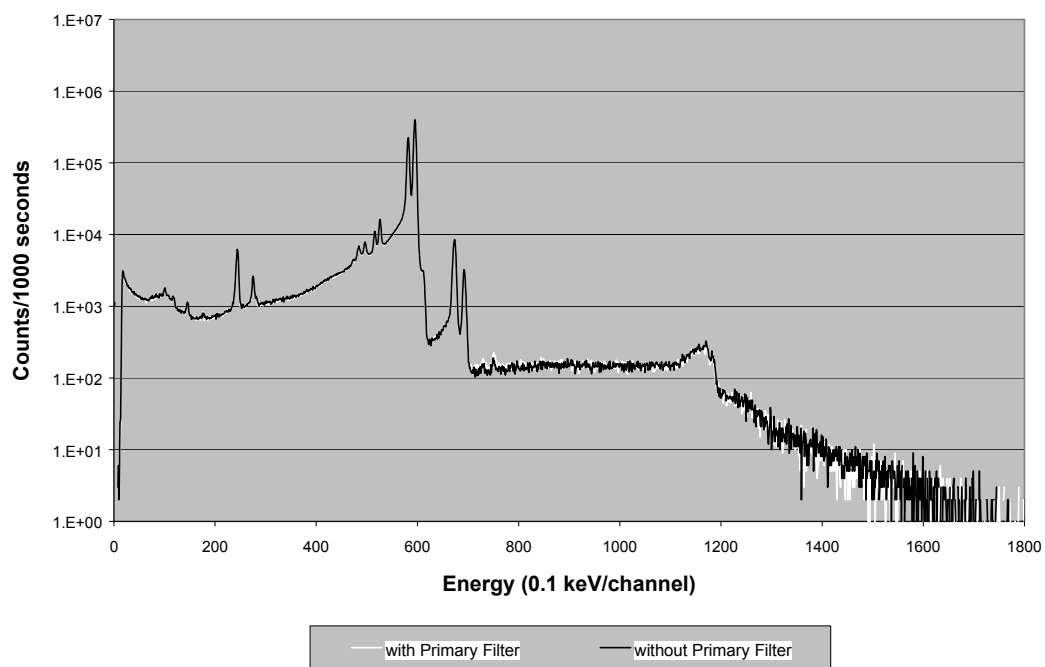


Figure 7.7b. Effect of Primary Filter on 59.3-keV K-Fluorescence Spectra

Beta Source Upgrade

Characterization of a new ^{204}Tl source continued in CY 2000. The source (318-360) was procured during CY 1999 to help reduce exposure times and the heavy demand these times place on the beta irradiation facility. It is encapsulated in a total of 9.2 mg/cm^2 of composite acrylic and Kapton, which is slightly different than the source it was designed to replace (318-192). The older source 318-192 was encapsulated in a total of 7.6 mg/cm^2 composite glass and Kapton. The originating source material was also specified by the manufacturer to be of lower specific activity than the older source, requiring a more substantial quantity of material to attain the desired activity. Because these two geometry considerations were observed as potential influences on the beta energy spectrum output by the source, several intercomparisons were planned using available dosimetry. In addition, routine characterization of the 20.7 mg/cm^2 transmission ratio and field uniformity were planned and performed to augment the CY 1999 measurements of maximum residual energy (E_{res}). The transmission ratio was found to be 0.78, which was well within the 0.80 ± 0.05 required tolerance, but less than the ratio of 0.838 for source 318-192.

Initially, it was anticipated that the new source would be configured with the same flattening filter used with the older source. As such, E_{res} measurements in CY 1999 were conducted with this configuration. An intercomparison was conducted in CY 2000 using chipstrate dosimeters encased within a special holder equipped with multiple thicknesses of aluminum filtration. Using this “multi-element beta dosimeter,” exposures were obtained with the older source, 318-192, and the newer source, 318-360. It was anticipated that results from this comparison could be used to provide the data necessary to predict the differences in response of lightly filtered dosimetry configurations and, if necessary, to serve as the basis for making minor adjustments to analysis algorithms. The results of this comparison are shown in Figure 7.8.

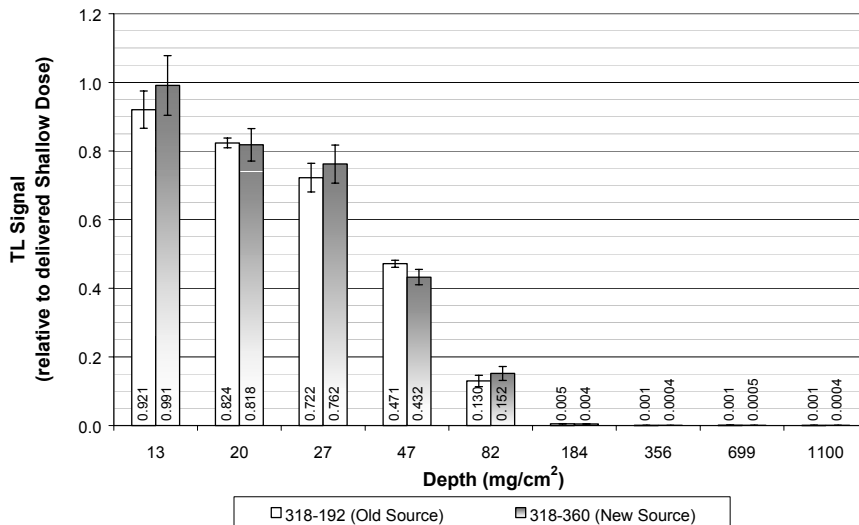


Figure 7.8. Comparison of New and Old ^{204}Tl Source Transmission (Measured through aluminum in 40 mg/cm^2 LiF)

Field uniformity measurements, using a thin-window, AIC, GM detector, and alumina film, were initiated in this configuration. Large disparities in results prevented a consensus of the field uniformity was not attainable. It was also determined that the alumina film did not have the necessary precision to resolve the field uniformity. Upon further review of the configuration, it was suggested that the flattening filter may be hindering the resolution of the uniformity, and possibly contributing to an intensified non-uniformity, because the penumbra from the filter appeared to bisect several measurement points. Based on this observation, it was decided to discontinue the use of the flattening filter in association with this newer source. As a result, calibration and characterization measurements were planned and initiated for the unfiltered configuration.

During the course of these subsequent measurements, source 318-192 was found to be losing encapsulation integrity, which mandated an immediate removal from service. Consequently, it would not be possible to conduct direct intercomparisons of the new source without the flattening filter against the older source. A recalibration of source 318-360 resulted in a shallow absorbed dose rate approximately 60% higher than the filtered configuration. E_{res} measurements in CY 1999 had demonstrated that the source was not encapsulated excessively and, because removing the flattening filter would be anticipated to increase the residual maximum energy, it was decided to postpone reassessment of this parameter until later. A more critical parameter was the 20:7-mg/cm² transmission ratio. Measurements were conducted using polyethylene terephthalate absorbers resulting in a ratio of 0.842. This represented an increase of less than 0.5% of the value determined for the older source 318-192, and within the 0.80 " 0.05 required tolerance specified in DOE/EH-0027 (DOE 1986b) and ANSI/HPS N13.11-1993 (ANSI 1993).

The source was implemented for irradiations and instrument characterizations in early October 2000; however, further characterization measurements are planned for 2001. These include an intercomparison of the transmission properties with and without the flattening filter, using the multi-element beta dosimeter, and an assessment of the maximum residual energy.

7.3 Program Assessments

Five audits/assessments were performed during 2000, all of which reviewed, in part, facets of the RS&C program. In chronological order these included, a self-assessment performed in accordance with the CR&A-specific procedure AP-0003, *CR&A Assessments and Problem Reporting*; an audit by two of PNNL's offsite DOE clients in reference to DOE/ID-12105, *Quality Assurance Manual for the Department of Energy Laboratory Accreditation Program for Personnel Dosimetry Systems* (DOE 1997b); an onsite assessment by NIST on behalf of NVLAP in reference to the criteria of NIST Handbook 150, *National Voluntary Laboratory Accreditation Program—Procedures and General Requirements* (NIST 1994; this handbook reiterates the "General requirements for the competence of calibration and testing laboratories" section of ISO Guide 25 (ISO 1990) as well as NVLAP interpretations of ISO Guide 25 via ANSI/NCSL Z540-1-1994 [draft]); and an assessment by a private client who conducts work on the Hanford Site.

These assessments, identified 16 items for corrective action with the CR&A internal tracking system. Of these items, nine were rated as observations and seven as noncompliance issues. None were classified as deficiencies, the most critical of the internal classifications. Table 7.4 identifies the general

Table 7.4. Summary of 2000 Audit Items

General Operational/Functional Area	Number of Internal Observation Reports		
	Observations	Noncompliance	Deficiencies
Organization and Management			
Quality System, Audit and Review	2	1	
Personnel			
Accommodation and Environment		1	
Equipment and Reference Material	3		
Measurement Traceability and Calibration	1	2	
Calibration and Test Methods			
Handling of Calibration and Test Items	1	1	
Records	1		
Certificates and Reports			
Outside Support Services			
Complaints			
Measuring and Test Equipment	1	1	
Software		1	

operational areas of these 16 items. All of the items identified in the table were entered into an Internal Observation Report tracking system and have been assigned recommended actions and expected completion dates, many of which will extend into 2001. The four external assessments have also been entered into the PNNL assessment tracking system.

There were no performance tests administered during the year.

7.4 Project-Related Professional Activities

Staff presentations and external professional activities during 2000 are listed in this section.

7.4.1 Presentations

Piper, R. K., J. C. McDonald, and R. A. Fox. 2000. "Proficiency Testing of Personnel Dosimeters at the Pacific Northwest National Laboratory." Presented at the 33rd Midyear Topical Meeting of the Health Physics Society, January 30 to February 2, 2000, Virginia Beach, Virginia.

Piper, R. K., M. K. Murphy, J. E. Tanner, A. K. Thompson^(a), and R. B. Schwartz^(a). 2000. "A Summary and Status of Traceability to National Standards for ²⁵²Cf Used at the Pacific Northwest National Laboratory." Presented at the 33rd Midyear Topical Meeting of the Health Physics Society, January 30 to February 2, 2000, Virginia Beach, Virginia.

(a) National Institute of Standards and Technology, Gaithersburg, Maryland 20899-8461

Piper, R. K. and R. A. Fox. 2000. “Dosimetry Testing at PNNL.” Presented at the Ninth Annual Meeting of the Council on Ionizing Radiation Measurements and Standards (CIRMS), October 30 to November 1, 2000, Gaithersburg, Maryland.

7.4.2 Publications

Piper, R. K., M. K. Murphy, J. E. Tanner, A. K. Thompson^(a), and R. B. Schwartz^(a). 2000. A Summary and Status of Traceability to National Standards for ²⁵²Cf Used at the Pacific Northwest National Laboratory. In *Proceedings of the 33rd Midyear Topical Meeting of the Health Physics Society*. Medical Physics Publishing, Madison, Wisconsin.

7.4.3 External Professional Activities

Fox, R. A., Member of the Working Group for ANSI N13.11, *Personnel Dosimetry Performance – Criteria for Testing*.

Murphy, M. K., Member of the ASTM Subcommittee E10.01, Radiation Processing Dosimetry, and Chair of the Task Group for *Standard Practice for Use of Photo-fluorescent Dosimetry Systems*.

(a) National Institute of Standards and Technology, Gaithersburg, Maryland 20899-8461

8.0 References

10 CFR 835. 1998. U.S. Department of Energy (DOE). "Occupational Radiation Protection." Revision 1. U.S. Code of Federal Regulations.

10 CFR 830. 2000. U.S. Department of Energy (DOE). "Nuclear Safety Management." U.S. Code of Federal Regulations.

American National Standards Institute (ANSI). 1972. *American National Standard Practice for Occupational Radiation Exposure Records Systems*. ANSI N13.6, New York.

American National Standards Institute (ANSI). 1975. *An American National Standard, Performance, Testing, and Procedural Specifications for Thermoluminescence Dosimetry (Environmental Applications)*. ANSI N545, New York.

American National Standards Institute (ANSI). 1978. *An American National Standard, Radiation Protection Instrumentation Test and Calibration*. ANSI N323, New York.

American National Standards Institute (ANSI). 1993. *An American National Standard, Personnel Dosimetry Performance—Criteria for Testing*. ANSI/HPS N13.11, American National Standards Institute, New York.

Freedom of Information Act, Public Law 89-847, July 4, 1966.

Health Physics Society (HPS). 1995. *An American National Standard, Performance Testing of Extremity Dosimeters*. HPS N13.32, Health Physics Society, McLean, Virginia.

International Commission on Radiological Protection (ICRP). 1977. "Recommendations of the International Commission on radiological protection." (ICRP publication 26). *Annals of ICRP*, 1:3, Elsevier Science, Inc., Tarrytown, New York.

International Commission on Radiological Protection (ICRP). 1979. "Limits for intakes of radionuclides by workers." (ICRP publication 30, part 1). *Annals of ICRP*, 2:3/4, Elsevier Science, Inc., Tarrytown, New York.

International Commission on Radiological Protection (ICRP). 1991. "1990 Recommendations of the International Commission on Radiological Protection." (ICRP publication 60). *Annals of ICRP*, 21:1-3, Elsevier Science, Inc., Tarrytown, New York.

International Commission on Radiological Protection (ICRP). 1994. "Human respiratory tract model for radiological protection." (ICRP publication 66). *Annals of ICRP*, 24:1-3, Elsevier Science, Inc., Tarrytown, New York.

International Standards Organization (ISO). 1984. *Reference Beta Radiations for Calibrating Dosimeters and Dosimeters and for Determining Their Response as a Function of Beta Radiation Energy*. ISO 6980, Geneva, Switzerland.

International Standards Organization (ISO). 1989. *Neutron Reference Radiations for Calibrating Neutron-Measuring Devices Used for Radiation Protection Purposes and for Determining Their Response as a Function of Neutron Energy*. ISO 8529, Geneva, Switzerland.

International Standards Organization (ISO). 1990. *General Requirements for the Competence of Calibration and Testing Laboratories*. Guide 25, Geneva, Switzerland.

International Standards Organization (ISO). 1996a. *X and Gamma Reference Radiation for Calibrating Dosimeters and Dose Rate Meters and for Determining Their Response as a Function of Photon Energy—Part 1: Radiation Characteristics and Production Methods*. ISO 4037-1, Geneva, Switzerland.

International Standards Organization (ISO). 1996b. *X and Gamma Reference Radiation for Calibrating Dosimeters and Dose Rate Meters and for Determining Their Response as a Function of Photon Energy—Part 3: Calibration of Area and Personal Dosimeters and the Measurement of Their Response as a Function of Energy and Angle of Incidence*. ISO 4037-3, Geneva, Switzerland.

Lynch, T. P., J. A. MacLellan, D. E. Bihl, R. K. Piper, M. L. Johnson. 2000. *Hanford Radiological Protection Support Services Annual Report for 1999*. PNNL-13238, Pacific Northwest National Laboratory, Richland, Washington.

National Institute of Standards and Technology (NIST). 1994. *National Voluntary Laboratory Accreditation Program, Procedures and General Requirements*. NIST Handbook 150. U.S. Department of Commerce, Washington, D.C.

Pinson, E. A., and W. H. Langham. 1980. "Physiology and Toxicology of Tritium in Man." *Health Phys.* 38 (1087-1110).

Privacy Act, 44 Federal Regulations 510 777 (1974).

Scherpelz, R. I., J. J. Fix, and B. A. Rathbone. 2000. *Validation of Hanford Personnel and Extremity Dosimeters in Plutonium Environments*. PNNL-13136, Pacific Northwest National Laboratory, Richland, Washington.

Sula, M. J., E. H. Carbaugh, and D. E. Bihl. 1991. *Technical Basis for Internal Dosimetry at Hanford, Rev. 1*. PNL-6866 R.1, Pacific Northwest National Laboratory.

U.S. Department of Energy (DOE). 2000. *Environment, Safety and Health Reporting Manual*, DOE Manual 231.1-1 Change 2, Washington, D.C.

U.S. Department of Commerce/National Bureau of Standards (DOC/NBS). 1982. *Proceedings for Calibrating Neutron Personnel Dosimeters*. NBS Special Publication 633, Washington, D.C.

- U.S. Department of Commerce. 1994. *National Voluntary Laboratory Accreditation Program - Procedures and General Requirements*. NIST Handbook 150-4, Gaithersburg, Maryland.
- U.S. Department of Energy (DOE). 1986a. *Handbook for the Department of Energy Accreditation Program for Personnel Dosimetry Systems*. DOE/EH-0026, Washington, D.C.
- U.S. Department of Energy (DOE). 1986b. *Department of Energy Standard for the Performance Testing of Personnel Dosimetry Systems*. DOE/EH-0027, Washington, D.C.
- U.S. Department of Energy (DOE). 1996. *Implementation Guide for Use with 36 CFR Chapter XII - Subchapter B Records Management*. DOE G 1324.5B, Washington, D.C.
- U.S. Department of Energy (DOE). 1997a. *Environment, Safety and Health Reporting*. DOE Order 231.1-1 Change 2, Washington, D.C.
- U.S. Department of Energy (DOE). 1997b. *Quality Assurance Manual for the Department of Energy Laboratory Accreditation Program for Personnel Dosimetry Systems*. DOE/ID-12105, Washington, D.C.
- U.S. Department of Energy (DOE). 1999a. *Internal Dosimetry Program Guide*. DOE G 441.1-3, Washington, D.C.
- U.S. Department of Energy (DOE). 1999b. *DOE Standard Internal Dosimetry*. DOE-STD-1121-98. Washington, D.C.
- U.S. Department of Energy (DOE). 1999c. *Occupational Radiation Protection Record-Keeping and Reporting Guide*. DOE G 441.1-11, Washington, D.C.
- U.S. Department of Energy (DOE). 2000. *Environment, Safety and Health Reporting Manual*. DOE Manual 231.1-1 Change 2, Washington, D.C.

Distribution

**No. of
Copies**

**No. of
Copies**

OFFSITE

DOE EM-4
M. Gavrilas-Guinn
Radiological Control Program Advisor
Environmental Management,
U.S Department of Energy
1000 Independence Ave., S.W.
Washington, D.C. 20585

DOE EH-54
R. M. Loesch
U.S. Department of Energy
Mail Stop - 5142
19901 Germantown Rd
Germantown, MD 20874-1290

4 DOE Albuquerque Field Office

M. G. Knight
Radiological Control Manager
Battelle Pantex Plant
P.O. Box 30020
Amarillo, TX 79120

R. J. Blum
Mound Laboratory
EG&G
Mound Applied Technologies
P.O. Box 3000
Miamisburg, OH 45342

J. M. Graf
Los Alamos National Laboratory
P.O. Box 1663
Los Alamos, NM 87545

S. Baker
RMRS
Rocky Flats Plant
P.O. Box 464
Golden, CO 80402-0464

2 DOE Chicago Field Office

S. Layendecker
Radiological Control Section
Brookhaven National Laboratory
P.O. Box 5000
Upton, NY 11973

Manager, Radiation Protection
Argonne National Laboratory
9700 South Cass Avenue
Argonne, IL 60439

DOE Idaho Field Office

G. Courtney
LITCO
P.O. Box 4000
Idaho Falls, ID 83404

DOE Nevada Field Office

C. T. Bastian
Bechtel Nevada
P.O. Box 98521
Las Vegas, NV 89193

**No. of
Copies****2 DOE Oak Ridge Field Office**

J. S. Bogard
Oak Ridge National Laboratory
Martin Marietta Energy Systems, Inc.
P.O. Box 2008
Oak Ridge, TN 37831

J. B. Hunt
Y-12 Plant
Martin Marietta Energy Systems, Inc.
P.O. Box 2009
Oak Ridge, TN 37831

DOE San Francisco Field Office

C. T. Prevo
Lawrence Livermore National Laboratory
P.O. Box 808
Livermore, CA 94550

DOE Savannah River Field Office

K. W. Crase
Westinghouse Savannah River Company
Savannah River Plant
P.O. Box 616
Aiken, SC 29802

**No. of
Copies****ONSITE****5 DOE Richland Operations Office**

T.L. Aldridge	K8-50
W. M. Glines	A2-15
B. M. Pangborn	A5-17
R. M. Rosselli	A7-50
D. E. Trader	K8-50

4 Environmental Restoration Contractor

D. E. Gergely	H0-15
C. L. Hellier	X0-34
J. E. Tarpinian	H0-09
S. L. Winslow	L5-64

Hanford Environmental Health Foundation

S. M. McInturff	H1-77
-----------------	-------

2 Fluor Daniel Hanford

D. B. Ottley	H5-26
G. D. Perkins	H8-67

Washington State University (Tri-Cities)

R. Filipy	H2-52
-----------	-------

**No. of
Copies**

37 Pacific Northwest National Laboratory

D. E. Bihl (2)	P7-02
E. H. Carbaugh	P7-01
S. K. Ennor	K1-01
J. J. Fix	K3-55
M. E. Hevland (10)	P7-02
S. D. Dossett	P7-75
M. L. Johnson (2)	P7-01
J. L. Kenoyer	K3-55
M. P. Long	P7-28
T. P. Lynch (2)	B1-60
J. C. McDonald	K3-53
J. A. MacLellan	P7-01
R. K. Piper (2)	P7-03
K. H. Pryor	K8-34
B. A. Rathbone	P7-02
W. J. Apley	K9-01
K. L. Soldat	K3-53
Radiation Protection Historical	
Files (c/o M. A. Combs) (2)	P7-01
Information Release Office (5)	K1-06